

(19) World Intellectual Property Organization
International Bureau




(43) International Publication Date
17 January 2002 (17.01.2002)

PCT

(10) International Publication Number
WO 02/04049 A1

- (51) International Patent Classification⁷: **A61M 5/20**, 5/315
- (74) Agent: **McMASTER OBERIN ARTHUR ROBINSON & HEDDERWICKS**; Stock Exchange Centre, 530 Collins Street, Melbourne, VIC 3000 (AU).
- (21) International Application Number: PCT/AU01/00830
- (22) International Filing Date: 10 July 2001 (10.07.2001)
- (25) Filing Language: English
- (26) Publication Language: English
- (30) Priority Data:
PQ 8679 10 July 2000 (10.07.2000) AU
PQ 8908 24 July 2000 (24.07.2000) AU
PQ 8909 24 July 2000 (24.07.2000) AU
- (81) Designated States (*national*): AE, AG, AL, AM, AT, AU, AZ, BA, BB, BG, BR, BY, BZ, CA, CH, CN, CO, CR, CU, CZ, DE, DK, DM, DZ, EE, ES, FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MA, MD, MG, MK, MN, MW, MX, MZ, NO, NZ, PL, PT, RO, RU, SD, SE, SG, SI, SK, SL, TJ, TM, TR, TT, TZ, UA, UG, US, UZ, VN, YU, ZA, ZW.
- (84) Designated States (*regional*): ARIPO patent (GH, GM, KE, LS, MW, MZ, SD, SL, SZ, TZ, UG, ZW), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, CH, CY, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE, TR), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, GW, ML, MR, NE, SN, TD, TG).
- (71) Applicant (*for all designated States except US*): **MEDRAD, INC.** [US/US]; One Medrad Drive, Indiana, PA 15051-0780 (US).
- (72) Inventor; and
- (75) Inventor/Applicant (*for US only*): **SAVAGE, Rodney, Brian** [AU/AU]; 27 Park Road, Rydalmere, NSW 2116 (AU).
- Published:**
— with international search report
- For two-letter codes and other abbreviations, refer to the "Guidance Notes on Codes and Abbreviations" appearing at the beginning of each regular issue of the PCT Gazette.*

(54) Title: IMPROVEMENTS RELATING TO MEDICAL INJECTOR SYSTEMS

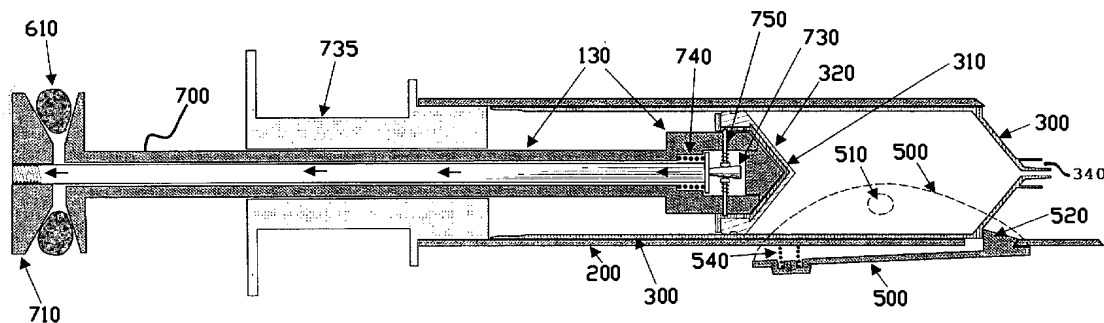

(57) Abstract: A medical injector system for injecting fluid from a syringe (300) into a patient, the syringe (300) having a barrel (300) and a plunger (310), the plunger (310) comprising an inner surface having an engaging portion (311) adapted to be releasably engaged by a plunger handle (130) which has a retention member (142) adapted to releasably engage the engaging portion (311) of the plunger (310); and a syringe holder comprising a cradle member (200) adapted to receive a barrel (300) of the syringe (300) and a pivotable catch (500) to releasably lock the syringe (300) in the cradle member (200).



WO 02/04049 A1

Improvements relating to Medical Injector Systems

Field of the invention

The present invention relates to medical injector systems for injecting medical fluids into a patient's vascular system.

5 Background of the invention

Medical injectors and syringes for injecting contrast media into a patient for imaging biological structures are known in the art. For example, U.S. Patent No. 4,677,980, issued to D. M. Reilly et al. on July 7, 1987, and entitled "Angiographic Injector and Angiographic Syringe for Use Therewith," which is assigned to the same Assignee as the
10 subject application, discloses an angiographic injector apparatus. The apparatus is designed for injecting contrast media into the vascular system of an animal, in which syringes are rear-loaded into a pressure jacket of the injector. More specifically, the apparatus comprises a rotatable turret which carries a pair of the pressure jackets and which is rotatable so that when one of the pressure jackets, into which a syringe has been
15 rear-loaded, is in an injection position, the other pressure jacket is in a position in which an associated syringe can be rear-loaded. Subsequently, when injection of contrast media from the first syringe is completed, the turret is rotated to move the first syringe to an unloading-loading position, with the second pressure jacket and the syringe concurrently being moved into the injection position.

20 In the apparatus disclosed in the '980 patent, a drive member of the angiographic injector can be drivingly connected to, or disconnected from, a plunger of a syringe at any point along the path of travel of the syringe plunger by a releasable mechanism. However, for the releasable mechanism to correctly operate, the syringe plunger must be properly oriented to mate with the injector piston. Further, during loading of the syringe on the
25 injector, the syringe must be correctly aligned within a respective pressure jacket to allow the syringe plunger and the injector piston to connect to and disconnect from each other.

An improved apparatus over the '980 patent apparatus is disclosed in U.S. Patent No. 5,383,858, issued to D. M. Reilly et al. on January 24, 1995, and entitled "Front-Loading Medical Injector and Syringe for Use Therewith," which is also assigned to the same
30 Assignee as the present application. In the apparatus described in the '858 patent, the

syringe is front-loaded onto, in at least one embodiment, a pressure jacket-less injector, overcoming one of the drawbacks of the '980 patent injector apparatus.

The injector described in the '858 patent has a first release mechanism for attaching and releasing the syringe from the injector. In addition, the apparatus includes a second release
5 mechanism that engages and disengages the injector piston from the syringe plunger. Upon rotation of the syringe, the syringe is attached to or released from the injector and, simultaneously, the plunger is attached to or released from the piston. The structure disclosed requires that the syringe be installed on the injector in a specific orientation so that the syringe can releasably engage the injector and, simultaneously, the plunger can
10 releasably engage the piston. In addition, as with the syringe disclosed in the '980 patent, during assembly the syringe plunger must be correctly oriented within the syringe.

Another injector apparatus is disclosed in U.S. Patent No. 5,300,031, issued to C. Neer et al. on April 5, 1994, and entitled "Apparatus for Injecting Fluid into Animals and Disposable Front Loadable Syringe Therefor." The '031 patent discloses various
15 embodiments of a pressure-jacketed injector wherein a syringe is loaded into and removed from an injector pressure jacket through an opening provided in the front end of the pressure jacket. To retain the syringe within the pressure jacket, for example, during an injection operation, the front end of the syringe is locked to the front end of the pressure jacket. To correctly connect the syringe to the pressure jacket, the syringe may only be
20 inserted into the pressure jacket in one orientation.

In each example discussed above, the syringe must be connected to the injector in a specific orientation to assure proper syringe mounting. Proper alignment is required to assure that the syringe may be operated properly during a medical imaging procedure. The required orientation, however, hinders rapid attachment and replacement of the syringe.
25 The required orientation may also increase the manufacturing assembly cost and complexity of the syringe.

Accordingly, while the above injector and syringe apparatuses have proven effective, a need has arisen for a simpler front-loading medical injector. More specifically, to facilitate further the loading operation, a need has arisen for a syringe that can be easily connected to
30 the injector without regard for the specific orientation of the syringe and/or syringe plunger. In addition, to simplify assembly of the syringe components, a need has arisen for

a syringe with a plunger that does not need to be oriented in a specific relation to the barrel or base of the syringe. Furthermore, to minimize the time required to prepare an injector for an injection procedure, a need has arisen for injectors providing automated features. There is a further need to add automated features which contribute to the safety of the patient, for example, by decreasing the chances of cross-contamination.

Medical fluids are normally packaged in containers or bottles, which have an elastomer bung (or cork) in the top. The bung can be pierced with a conventional needle or a plastic spike to draw fluid from the bottle into the syringe. However it is common practice to simply remove the bung, and draw up fluid into the syringe using a plastic cannula. This practice exposes the fluid to ambient microbes, and allows contamination, and thus increases the risk of undesirable infection of the patient. Certain vented spikes with special microbe filters have been developed to address this problem. However in use, the filling procedure is very tedious, and some fluid is often lost through the filter. Where large volumes are drawn into the syringe according to known methods, it can be very difficult to simultaneously hold the bottle inverted, and draw back the syringe.

Another important requirement when using syringe pumps to inject patients is to ensure that all air is purged from the system, including the tube, before it is connected to the patient. If this is not done, then it is possible that a bubble of air may be injected into the patient which can cause serious illness.

It has also been found that existing injector apparatus and injectors do not have features which discourage inadvertent re-use of syringes and associated tubes and spikes, which can result in the serious hazard of cross infections from one patient to the next.

Luer connectors are found on the outlet of most syringes used in medicine, and are well defined in International Standard ISO594. A locking thread is sometimes found associated with luer connectors, termed "luer locking", and are particularly used for higher pressure applications, where the thread assists closure and retention of the connections.

Flexible plastic tubing is used in many medical applications for conveying drugs, fluid, contrast etc between syringes and patients. The tubes are normally manufactured from flexible plastic, with luer connectors bonded to each end to facilitate secure and releasable male and female connections. Connectors are normally moulded from rigid plastic, having a luer outlet, with an cylindrical inlet sized to accept a close interference fit with the

relatively soft tube. The tubing is forced over (or inside) the cylindrical inlet end, and is traditionally bonded using solvent or cement adhesive. For higher pressure applications the bond must be very certain and secure to avoid bursting.

On occasions, the tubing may be attached permanently to the syringe, for example to
5 reduce manufacturing costs, reduce the chances of spilling contaminated fluids, or to protect the tip of the syringe from contamination. However bonding directly to syringes is rarely successful or certain because syringes are usually moulded from polypropylene. Some tubing materials are also difficult to bond. Moreover, bonding normally requires the use of powerful solvent cements such as cyclohexanone, or cyanoacrylates, both of which
10 release harmful vapours, and can leave unwanted residues.

In this specification, unless the contrary is expressly stated, where a document, act or item of knowledge is referred to or discussed, this reference or discussion is not an admission that the document, act or item of knowledge or any combination thereof was at the priority date:

- 15 (a) publicly available;
- (b) known to the public;
- (c) part of common general knowledge; or
- (d) known to be relevant to an attempt to solve any problem with which this specification is concerned.

20 **Summary of the Invention**

According to a first aspect of the invention, there is provided a syringe holder for a medical injector system comprising a cradle member adapted to receive a barrel of the syringe; and a pivotable catch to releasably lock the syringe in the cradle member wherein the catch is biased towards a first position and engages the syringe at the first position and disengages
25 the syringe at a second position.

By providing a pivotable catch to releasably lock the syringe, it is possible to enable front-loading of syringes into the syringe holder by removing the requirement of a front wall on the cradle. A person skilled in the art will appreciate that the catch surface can be varied in length to engage a larger (or smaller) amount of the syringe surface.

According to a particularly preferred embodiment, the syringe holder further comprises a positioning device located on the cradle member to locate one end of the syringe in a predetermined location in the cradle member.

5 According to one preferred embodiment, the cradle member is a sleeve and surrounds the barrel of the syringe. Preferably such a sleeve is adapted to support the syringe against expansion under pressure to provide support against internal pressure during expulsion of fluid. This allows the wall thickness of the barrel to be reduced, thereby saving manufacturing costs.

10 According to another preferred embodiment, the catch mechanism engages a front shoulder of the syringe. Preferably the catch engages the syringe through a hole defined in the cradle or sleeve.

According to another preferred embodiment, upon insertion of the syringe barrel into the cradle or sleeve, a front portion of the catch engages a corresponding front portion of the syringe, to thereby retain the syringe within the cradle or sleeve. To remove the syringe
15 from the cradle or sleeve, a rear portion of the catch is depressed, causing the front portion to disengage from the syringe barrel.

The syringe may be loaded through the front end of the pressure sleeve by simply sliding until the catch locks automatically. This manner of loading from the front is simple, requiring no twisting or conscious locking action by the operator. The syringe may also be
20 simply released by pressing the syringe release button, and withdrawing the syringe forward. The catch may be part of the cradle member to enable assembly and replacement to / from the sleeve, for cleaning or renewal.

The syringe holder is preferably fabricated from transparent hard plastic, and comprises a plain cylinder having an open end, cut off at an angle of approximately 50 degrees to
25 enable easy insertion of the syringe. Construction from transparent material provides unobstructed vision of the syringe and its contents, particularly of the forward end where all air must be purged following filling. Typically the sleeve is of one piece construction (optionally including a spring), and low cost to manufacture by fabricating from plain stock tubing, or moulding process.

The rear end of the sleeve is preferably fixed (preferably releasably for cleaning) to the injector, aligned co-axially with the injector plunger – this enables the syringe to be removed from the injector at any time without fear of the plunger touching the inside of the syringe (and thereby possibly contaminating it). Volume graduations may be printed onto the sleeve of the holder, and are thereby not required on the syringe.

The syringe is loaded rear first into the front of the holder, which forms a close fitting sleeve supporting the syringe against expansion under the high pressures endured with injectors. The holder preferably has a square notch towards the front which allows access for, and supports the syringe catch whilst under load. Two round holes in the sleeve are preferable to act as hinge sockets for the catch.

Preferably the catch is moulded as a partial cylinder shape from a hard flexible plastic, and has 2 opposing hinge posts which snap into corresponding holes in the sleeve. For replacement or cleaning purposes the catch assembly can be removed by simply spreading the sides apart until the hinge posts clear their respective holes.

According to another preferred embodiment, the cradle member has a biasing member to partially eject the syringe from the cradle member upon release of the catch. Preferably the biasing member upon insertion of the syringe barrel is actuated, thereby biasing the barrel towards a partially ejected position so that the barrel is partially ejected from the sleeve upon release of the catch. Preferably the self-ejecting mechanism (created by the biasing member) comprises a spring and is preferably located at the rear of the sleeve, which upon insertion of the syringe barrel is compressed.

According to another preferred embodiment, the biasing member is adapted to engage and minimize rotation of the syringe.

According to another preferred embodiment, the biasing member is adapted to operate or engage an optical sensor or switch, which advises the injector control unit of the presence of a syringe.

According to one embodiment, the cradle member may be permanently attached to the injector, rather than removed each time the syringe is replaced, thereby improving convenience, and reducing the chance of dropping and soiling the sleeve.

An extension tube can be permanently attached to the syringe. Being front loaded, the associated connecting tube need not be disconnected from the syringe following injection, reducing the risk of spilling contaminated blood.

5 The catch may be of any suitable shape. According to a particularly preferred embodiment, the front shoulder of the syringe is of a complimentary shape to an engaging portion of the catch. The catch surface may be longer (such as about half of the syringe circumference or substantially co-extensive with the cradle) to more easily retain the syringe on the injector.

10 The engaging portion of the catch may be of any suitable shape. According to certain preferred embodiments, it is wedge shaped, concave or convex. Optimally the catch mechanism is wedged against the forward edge of an associated notch in the syringe sleeve, transferring most of the load onto the notch (and thus the sleeve and injector), and not on the catch hinges.

15 As the syringe is loaded into the sleeve the syringe catch is pushed aside. Once the syringe is fully home the front of the syringe clears the catch, and the catch latches due to tension from the spring under the button, forming a fixed stop in front of the front rim of the syringe. If the catch is a dovetail shape, then it is unlikely to partially close, and even if it were to, any tension from the syringe would draw the dovetail catch closed.

20 During injection the forward force of the syringe is borne by the catch. Such a catch forms a dovetail between the syringe and the notch in the sleeve, so that the catch cannot be released, nor slip whilst under load.

According to another preferred embodiment the holder or the injector system comprises an illumination member to illuminate the syringe holder. The illumination member may be mounted, engaged or attached to any suitable component of the holder or injector system
25 Preferably it is mounted to the holder. According to another preferred embodiment, it is mounted to the injector and preferably in the nose of the injector. The illumination member may be of any suitable type or light source. It may be a lamp, or globe, it may be a Light Emitting Diode (LED). Preferably the illumination member is placed at the exposed rear end of the holder cradle member or sleeve so that some of the light is received and transmitted
30 along the walls of the cradle member or sleeve. As with any thin, dense, transparent material, most of the received light is internally reflected longitudinally, as well as laterally, producing a

diffused glow at the front end of the cradle member or sleeve. Preferably the cradle member or sleeve has a bevelled front end of the sleeve which is preferably frosted (for example, it may be sanded) to achieve maximum diffusion, and is therefore visible from a wide angle. Any suitable light source may be used, but they are preferably focused or reflected so that most of
5 their output is projected towards the sleeve. The provision of an illumination member has a variety of useful benefits. In particular it will assist visualisation of the holder and other components in radiography rooms which are dimly lit for certain procedures.

According to another preferred embodiment, the syringe holder comprises an engagement portion to enable simple releaseable engagement with a medical injector. Preferably the
10 engagement portion comprises a locking member and preferably the locking member comprises a slot or a pin.

Such a removable syringe holder provides benefits including:

- (a) Allows the syringe holder to be easily removed by the operator for cleaning;
- (b) Allows easy replacement if worn or damaged;
- 15 (c) Enables the injector to accept a different size or type of syringe; and
- (d) Removal for shipment reduces the overall packaging size.

To engage a syringe holder according to the present embodiment with the injector (or injector nose), the sleeve is first inserted into the nose and with gentle inwards pressure, rotated until the bayonet grooves engage the bayonet posts. At this point the holder fully
20 enters the nose, and the holder is rotated clockwise to lock. The bayonet groove and post sets may be spaced evenly around the circumference, or they could also be oriented at matching odd angles so that the holder can only engage in a particular orientation. Preferably there is also provided a Fluid Seal & Friction Device. It may be a simple O-ring or wiper ring, and has two important roles:

- 25 (a) prevent fluids from entering the injector;
- (b) provide a friction means to decrease the possibility of inadvertent removal of the syringe holder.

According to a particularly preferred embodiment, the syringe holder comprises a blocking member to regulate disengagement of the holder with the medical injector. Preferably the

blocking member stops disengagement of the holder with the medical injector if a syringe is present in the holder. According to a particularly preferred embodiment, the blocking member stops disengagement of the holder with the medical injector if the plunger is not in a particular position. According to another particularly preferred embodiment, the
5 blocking member stops disengagement of the holder with the medical injector if the plunger is not in a sufficiently retracted state.

A blocking member according to the present invention if in the form of a lock post is preferably positioned adjacent to the syringe sensor and therefore the syringe holder cannot be removed whilst a syringe is installed, nor during an injection. Additionally, a syringe
10 cannot be installed unless the holder is locked fully (for example by clockwise rotation). This embodiment is particularly useful in the absence of a sensor to verify syringe presence. It will be appreciated that the holder according to this embodiment could not be attached if a syringe were already installed.

Preferably a lock post according to this embodiment is of similar width to, and mounted on
15 the same axis as the syringe flag form of the sensing system according to this invention (discussed below). As the holder is attached, the flag almost touches it when the bayonet slots are fully engaged with the bayonet posts (without rotating). According to this embodiment, in the mounted position, with a syringe installed and the flag pushed back, the holder cannot be rotated the wrong way (in the present case anti-clockwise).

20 According to a further aspect of the invention, there is provided a hub for a syringe for use with a medical injector system, comprising an outer surface adapted to slidably engage with a barrel of the syringe, and an inner surface having a substantially annular engaging portion adapted to be releasably engaged by a plunger to permit the hub to be selectively withdrawn along the barrel by the plunger.

25 By providing a hub with these features, a number of benefits can be obtained which relate to the efficiency of use and safety of the patient to be injected as set out below. Since the plunger remains on the injector, then a syringe having a hub according to the present invention can be fitted over it and thus enable front loading which is much quicker. In addition, front loading avoids the requirement of detaching any extension tubing from the
30 front (nearest the patient) of the syringe and thus decreases the chance of spilling blood which may be contaminated.

The engaging portion may be of any convenient conformation for example, it may be a cavity, a groove or a ridge. Where the engaging portion is a groove, the groove may define a semi-circular cross-section or the groove may extend at least partially along the circumference of the inner surface of the hub. Preferably there are no protrusions from the rear of the hub to impede its movement along the barrel of a syringe.

A hub of this type has many advantages. The thin and uniform wall thickness is ideally suited to injection moulding and provides economies of manufacture in light of the reduced material volume required, the reduced moulding cycle time and the requirement for only simple tooling.

According to one preferred embodiment, the inner surface of the hub is complementary in shape to an outer surface of the plunger. Preferably the inner surface of the hub comprises an interior hollow that contacts the plunger. Such an arrangement allows for a form fit which has the advantage of providing a reinforcing effect to the hub. This allows the wall thickness of the hub to be reduced as compared with hubs of the prior art, thus contributing to the abovementioned economies of manufacture. Preferably the plunger has a tapered front end, which is inherently "self centering" as it engages the hub. This also provides uniform, coaxial support of any seal associated with the hub and improved sealing as compared with hubs of the prior art - particularly at the high pressures used in certain medical injectors. At high pressures the hub can be forcibly expanded to improve its seal against the syringe barrel.

The preferred resilient nature of the hub advantageously provides for positive-fit or force-locking of the retention members at the engagement portion and enables considerable force to be applied when the contents of the syringe are expelled at high pressures.

The hub may also be adapted to engage a seal associated with at least a portion of an outer surface of the hub, or alternatively, the hub may perform the function of a seal. The hub or seal may be used in combination with an o-ring. Preferably the seal, whether it is separate from the hub or not, has an extended leading edge to increase the efficiency of the seal under pressure.

According to a further aspect of the invention there is provided a plunger for a syringe for use with a medical injector system, the syringe having a barrel and a hub slidingly engaging the barrel, the plunger comprising a retention member adapted to releasably

engage a substantially annular engaging portion on an inner surface of the hub to permit the hub to be selectively withdrawn along the barrel by the plunger.

As discussed above, by providing a plunger disposed within the housing and comprising a retention member to releasably engage the engaging portion of the hub, it is possible to
5 utilize a single plunger associated with the injector system with multiple syringes, each with a hub according to the present invention. The retention member enables the plunger to engage and lock onto the hub and thereby drive it either backwards or forwards along the syringe barrel to draw fluid into or out of the syringe. Preferably there is more than one retention member.

10 A retention member according to the present invention may be of any suitable type. Preferably the retention member is mechanically and/or electrically releasably engaged with the hub. According to this embodiment, it is possible to cause the plunger to engage the hub by actuation (as opposed to automatic engagement by pushing or forcing the plunger into the hub). This creates greater control over locking and release of the hub by
15 the plunger, which is important for applications where the plunger movement is controlled electronically. For example, it is particularly advantageous to be able to release the hub at the most front (outlet) portion of the syringe after expulsion of fluid since this will minimize the possibility of re-use of the syringe. According to another preferred embodiment, the releasable engagement is at least partly actuated by a weight mechanism.

20 According to one preferred embodiment, the releasable engagement is actuated by retraction of the plunger. According to another embodiment, the plunger may be adapted with a weight mechanism such that the retention members are activated (for example, they may protrude from the plunger) when the plunger is in a particular orientation.

According to another preferred embodiment, the releasable engagement occurs
25 automatically on retraction of the plunger and automatically releases the hub during and following forward movement of the plunger, leaving the syringe unlocked following an injection, free to be removed safely. Such an embodiment operates as follows:

The nose portion of the actuation member (the Cone) is attached to the actuation member, which in turn is fixed to the plunger drive. The plunger is driven backward to draw up (fill)
30 a syringe, then forward to expel the syringe. It should be noted that the plunger is slidingly engaged with the actuation member, but with a limited free play. Note also that free sliding

of the plunger may also be somewhat reduced by a Friction Seal. According to this embodiment, whenever the plunger drive and actuation member reverse direction, the plunger does not move until the actuation member has traveled some millimeters, and the hub lock mechanism changes state.

- 5 The actuation member slides inside the momentarily stationary plunger. The drive and actuation members move forward relative to the plunger and lock pins, allowing them to retract and unlock the syringe. The plunger does not move (due to friction of the Seal) until the shoulder of the plunger drive strikes the rear of the plunger, at which point the hub begins advancing, expelling the syringe. The purpose of unlocking the hub is to allow
10 removal of the used syringe following an injection.

When the plunger begins to retract again the plunger (and hub) is momentarily stationary - the Cone retracts relative to the Lock Pins, extending them to lock the hub onto the Plunger. A shoulder on the actuation member then strikes the Inner Shoulder of the Plunger, retracting it and the hub back for filling etc.

- 15 Hence this system automatically ensures that the hub is either locked or unlocked at the appropriate time, avoiding inconvenience and enhancing safety of the injector - for the operator and the patient. Of course, a controller associated with the injector may be programmed to allow for the inherent "free play" whenever the plunger reverses direction.

Benefits of this embodiment include:

- 20 (a) Whenever the plunger is advanced the lock pins automatically immediately retract, allowing the plunger to freely enter the hub, regardless of whether the hub had already engaged the plunger. With a gravity operated lock system the piston has to engage the plunger before the head is tilted up (and locked).
- (b) With a gravity operated system the head has to be tilted downward to unlock, and
25 the syringe can then be removed.
- (c) The syringe hub can be retracted at any time, including to test the patency of a needle. Previously pre-filled syringes can easily be "topped up" at any time. Previously pre-filled syringes can now be purged with the head oriented upwards (This was not possible with the gravity lock system because the lock pins

automatically extend when oriented vertically, but the plunger will not yet have engaged the hub).

- (d) The hub is always left unlocked following an injection, allowing safe removal of the syringe at this logical point in the injector sequence.
- 5 (e) The hub is automatically and immediately locked whenever the plunger is retracted, ensuring the hub will be pulled back.
- (f) New syringes may have the plunger assembled and left in any position along the barrel (for the previously described Gravity Lock system the hub must be located at the very rear of the barrel).
- 10 (g) This concept is robust and reliable.

According to another preferred embodiment, the retention mechanism is biased to lock only when the syringe is oriented vertically (as necessary when filling & purging), and is automatically unlocked in the injection position. This is desirable to prevent drawing up blood into the syringe, or its re-use. Given certain controls over plunger movement this
15 mechanism can form part of an injection system which can minimise or prevent re-use of a syringe, thereby helping prevent cross infection from one patient to the next. For example, given the following scenario:

New syringes are usually supplied with the retention members and hub in the fully retracted position. Syringes are loaded through the front end of a fixed retaining sleeve
20 (which is part of the holder) of the injector, which aligns the syringe and hub with the plunger of the injector. The injector can only inject following filling, and with the syringe oriented such that its front (outlet) portion is at the same level or below its back (furthest from the patient) portion, that is, the syringe is in a horizontal or down orientation to avoid injecting any residual small amounts of air. With this system the plunger is automatically
25 retracted immediately after completion of an injection, thereby leaving the used hub in the expelled position. The plunger can only be retracted on demand if the syringe is oriented vertically. For the injector plunger to lock into the hub, the plunger must be fully engaged with the hub before the retaining members are extended (this system extends the retaining members as the plunger is tilted from the horizontal to the vertical). As a new syringe is
30 loaded, the hub will, by default, engages the plunger of the injector and as the injector is

subsequently tilted up a weight mechanism, such as a weighted rod slides backward due to gravity, and thereby actuates the retention member to secure the hub onto the plunger. The injector can now retract the plunger, and fill the syringe by drawing fluid down into it.

5 If a used (even partially expelled) syringe were loaded into the injector, its hub would, by default, be positioned forward of the retracted plunger and cannot engage with it. When the injector is tilted up (thus tilting the front of the syringe up), the retention members extend, but do not secure the hub. Hence the hub cannot be drawn back and the syringe can not be re-filled.

10 As syringes for use with and according to the present invention do not have their own plunger, there is no protrusion from the rear of the syringes. Therefore there is little danger of dislodging the hub in transit and during handling. (As described above, the syringe is best assembled with the hub as far back as possible).

According to another preferred embodiment, the retention member is biased away from engagement with the hub.

15 In another preferred embodiment, the retention member comprises an actuation member disposed at least partially within a bore defined in the plunger and a locking member is located at or adjacent one end of the retention member and/or plunger, the locking member being movable by the retention member into or out of engagement with the engaging portion of the hub.

20 The retention member may comprise any suitable member, but preferably it is a cam or a cone. Preferably the cam or cone is moved into and out of the bias position by a weight mechanism which causes the protrusion of the retention member in accordance with a given orientation of the plunger.

25 According to another preferred embodiment, the actuation member has a rod portion and a nose portion and the locking member is, in the unlocked position, located between the plunger and the nose portion. Preferably the actuation member is movable longitudinally along the bore in the plunger and preferably the retention member comprises a pin. In a particularly preferred embodiment, there is more than one pin.

30 According to a still further preferred embodiment, the plunger is adapted for manual filling of the syringe. By adapting the plunger for manual filling of the syringe, it is possible to

hand fill syringes without the need to load them in the injector. This has the benefit of allowing a number of syringes to be pre-filled and thereby speed up the process of changing from one syringe to the next, and allows filling of a new syringe when the injector is injecting a previous patient. In addition a plunger according to this aspect of the invention can be used to hand fill a series of syringes and then be placed into the injector for injection of patients, thereby minimizing the need for separate hand filling devices.

Preferably the plunger according to this aspect of the invention is sufficiently shorter than the barrel of the syringe such that it can not reach the hub when the hub is located at the front most portion of the syringe barrel. In other words, the plunger is slightly shorter than the full syringe stroke, thereby is incapable of engaging the hub after the syringe has been used (assuming the syringe was fully expelled). A plunger / plunger device according to this aspect of the invention will decrease the chances of re-use of syringes (and thus cross-contamination) by being incapable of grasping and retracting the hub within the syringe. Preferably the plunger is sufficiently shorter than the barrel of the syringe such that it can not reach the hub when the hub is located at the front most portion of the syringe barrel.

According to a further aspect of the invention, there is provided a plunger for a syringe for use with a medical injector system, the syringe having a barrel and a hub slidingly engaging the barrel, the plunger comprising a retention member adapted to releasably engage an engaging portion of the hub to permit the hub to be selectively withdrawn along the barrel by the plunger; and a sensor to detect a level of engagement between the plunger and the hub.

A sensor according to this aspect of the invention may be any suitable sensor, such as a mechanical, electromagnetic or light sensor. Preferably the sensor detects full engagement between the plunger and hub. Where the sensor is a light sensor, then preferably it comprises a fibre optic cable.

According to one preferred embodiment, an optic fibre is embedded inside the plunger having one end exposed and flush with the surface of the plunger, and carefully positioned so that the end is masked by the hub just as the plunger fully engages the hub. The flexible fibre is routed out the rear end of the plunger, and via a suitable slack loop the other end of the fibre is connected to a photo detector which can respond to light transmitted through the fibre. Note that the plunger moves back and forth often, and so the fibre is a convenient

and reliable means for communicating with the plunger. For the present invention the hub is made from opaque material, whilst the syringe barrel is transparent.

The injector is always used in a normally illuminated environment, and hence the fibre normally "sees" light (in the absence of a syringe hub). Of course, if the room lights are
5 inadequate, the plunger can be illuminated by the injector with visible or infrared light. As the plunger engages the hub, the ambient light is cut off from the tip of the fibre, signalling the photo detector and Control Unit.

This device detects when the plunger has entered the piston, and when connected to the Injector Control Unit, provides the following benefits and enhancements:

- 10 (a) where the syringe has been pre-filled, the plunger must be engaged with the hub prior to initiating the injection, so that when the injector is started the hub begins expelling immediately. This device enables the injector to safely and accurately engage the hub and plunger, without pushing the hub (which could cause unwanted waste and mess).
- 15 (b) If used in association with the syringe sensing system described below, where the syringe has been pre-filled or the hub is not fully retracted, the plunger can automatically advance to engage the hub, then stop accurately.
- (c) Where an automatically (for example, electronically) controlled hub and plunger engagement mechanism is employed, this sensor can be used to indicate that the
20 piston retention mechanism is ready for locking.
- (d) If used in association with a gravity locked plunger and a syringe presence sensor, this device can signal whether the hub is fully retracted when the syringe is first loaded, thereby confirming whether the syringe is new, or alerting the operator that the syringe has been used and may be contaminated.
- 25 (e) The device can also generate a signal if the piston becomes detached during retraction or filling.

According to a still further aspect of the invention there is provided a device for manually filling a syringe for use with a medical injector system, the syringe having a barrel and a hub slidably engaging the barrel, the device comprising a plunger and a retention member

adapted to releasably engage an engaging portion of the hub to permit the hub to be selectively withdrawn along the barrel by the plunger.

Such a device enables the operator to hand fill syringes without the need to load them in the injector. This has the benefits of allowing a number of syringes to be pre-filled and thereby speed up the process of changing from one syringe to the next, and allows filling of a new syringe when the injector is injecting a previous patient. In addition a device according to this aspect of the invention can be used to hand fill a series of syringes and then be placed into the injector for injection of patients, thereby minimizing the need for separate hand filling devices.

- 10 Preferably a device according to this aspect of the invention is sufficiently shorter than the barrel of the syringe such that it can not reach the hub when the hub is located at the front most portion of the syringe barrel. In other words, the device is slightly shorter than the full syringe stroke, thereby is incapable of engaging the hub after the syringe has been used (assuming the syringe was fully expelled). A device according to this aspect of the invention will decrease the chances of re-use of syringes (and thus cross-contamination) by being incapable of grasping and retracting the hub within the syringe. Preferably the device is sufficiently shorter than the barrel of the syringe such that it can not reach the hub when the hub is located at the front most portion of the syringe barrel.

- 20 Preferably the retention member is mechanically and/or electrically releasably engaged with the hub.

According to another preferred embodiment, the releasable engagement is at least partly actuated by a weight mechanism. According to another preferred embodiment, the releasable engagement is actuated by retraction of the plunger. Preferably the retention member is biased away from engagement with the hub.

- 25 According to a further preferred embodiment the retention member comprises an actuation member disposed at least partially within a bore defined in the plunger and a locking member is located at or adjacent one end of the retention member and/or plunger, the locking member being movable by the retention member into or out of engagement with the engaging portion of the hub. The retention member may be of any suitable form, it may be a cam, it may be a cone.
- 30

According to another preferred embodiment the actuation member has a rod portion and a nose portion and the locking member is, in the unlocked position, located between the plunger and the nose portion. Preferably the retention member comprises a pin.

According to another aspect of the invention, there is provided a method for hand filling a syringe comprising a hub according to the present invention and a device for hand filling according to the present invention comprising the steps of; (i) introducing the device into the syringe barrel and engaging the device with the inner surface of the hub (ii) activating the device such that the retention member engages the engaging portion of the hub; and (iii) withdrawing the engaged hub along the syringe barrel whilst drawing liquid into the syringe.

According to a further aspect of the invention, there is provided a syringe for use with a medical injector system including a hub as described above.

According to a further aspect of the invention, there is provided a syringe for use with a medical injector system including a plunger as described above.

In a particularly preferred embodiment of a syringe according to this aspect of the invention, it comprises a plunger as described above and a hub as described above.

According to another aspect of the invention, there is provided a sensing system for use with a medical injector system comprising a sensing member to detect the presence of a syringe holder associated with the medical injector system. The sensor may be of any suitable type such as a light sensor, mechanical sensor or electromagnetic sensor. Preferably it is a light sensor. Where the sensor is a light sensor, then preferably the sensing system further comprises a reflecting member to reflect light to the sensing member. The reflecting member may be associated with any suitable component, such as the syringe, or the injector system. The sensor system may alternatively comprise a light interruptor, contacts, or mechanical switch component.

According to one preferred embodiment, during assembly of the holder a syringe stop (or bush) and spring stop are normally fixed in place inside the holder by any suitable means such as cement, screws, or pins. Both stops have a small longitudinal groove in their outer surface to support a slidable syringe flag, which, together with the flag spring are held in place by the two stops. The compression spring is lodged between the rear fixed spring

stop and the flag tabs, thereby biasing the flag forward. With no syringe loaded the flag protrudes forward of the syringe stop, and its tabs lodge against the rear of the syringe stop. A secondary function of the syringe stop is to bear and centre the plunger, and prevent stray fluid around and/or from the syringe from entering the injector.

5 In brief, a sensing system according to this aspect of the invention can perform at least three functions:

1 Syringe ejector: According to one embodiment, the sensing system comprises a flag which is slidably mounted in a groove, and is biased forward by a flag spring. As the syringe is loaded into the holder the rear rim of the syringe strikes the flag,
10 pushing it rearward and compressing the flag spring until the tip of the flag is flush with the syringe stop. When the syringe catch is opened the syringe is partially ejected forward by the flag, making the syringe easier to grasp and remove.

2 Anti Rotation Device: Unlike most other syringe/holder arrangements, with the present invention the syringe can be rotated about its axis. When a tube is attached
15 to the syringe (after it has been loaded), the operator needs to twist the connection clockwise to engage and lock the connection to the syringe thread. To restrain the syringe from rotating it would ordinarily need to be held with the other hand, however the flag may perform this role. The forward tip of the flag is bevelled & sharpened, and thus can dig into the syringe and thereby decrease rotation of the
20 syringe.

3 Syringe Sensor: In association with the sensing system the flag detects the presence of a syringe in the holder. Reflective infrared sensors such as Sharp GP2L24 are readily available examples of sensors that may be used as part of the system. As the flag is pushed back by the syringe the reflective rear end of the flag
25 is detected by the sensor, which in turn may signal a controller associated with the injector system.

Electronic sensing of the syringe, coupled to a controller associated with the injector system enhances the functionality and safety of the injector. For example:

(a) To avoid cross infection from patient to patient it is important that the syringe is
30 replaced before the injector can allow a subsequent filling or injection.

- (b) Where a gravity operated plunger/hub locking mechanism is employed, the syringe should only be removed when the injector head is oriented horizontally (ie when the piston is unlocked) – if removal is attempted in the vertical orientation, the injector controller can alert the operator.
- 5 (c) In the case of an electrically operated piston lock, the injector controller can automatically lock following loading of a syringe.
- (d) As with any injector, the syringe should not be removed unless the hub is unlocked from the plunger (otherwise the hub could be separated from the syringe barrel, potentially spilling contaminated fluid or drug). In the case of certain of the
10 described embodiments the syringe is only able to be removed at the end of a forward (inject) stroke. Hence the controller must not allow retraction of the plunger until the sensor advises that the syringe has been removed following an injection.
- (e) With all syringe holders, to avoid accidental opening or failure during an injection
15 it is important that the device is fully locked in position before it can be used. If a syringe holder is not fully engaged with the injector system, it should be noted that the flag will not intersect the proximity sensor (preventing operation of the injector) until the holder is fully rotated to the locked position, and a syringe is present.

Similarly, a person skilled in the art will appreciate that configurations which do not utilize
20 a flag but instead utilize some other form of sensing mechanism will have the same and other benefits. Other benefits of a sensor system according to the present aspect of the invention include:

- (a) The sensitive electronic proximity sensor is fully protected from stray injection fluids which could damage or interfere with the sensor.
- 25 (b) Because the holder according to certain embodiments is able to be removed for washing, the sensor is not exposed to washing fluids.
- (c) The system is solid state (apart from the flag) and therefore robust & reliable.

According to a further aspect of the invention, there is provided a medical injector system for injecting fluid from a syringe into a patient, the syringe having a barrel and a hub

slidingly engaging the barrel, the hub comprising an inner surface having an engaging portion adapted to be releasably engaged by a plunger, the injector system comprising: (i) a plunger for driving the hub, the plunger comprising a retention member adapted to releasably engage the engaging portion of the hub; and (ii) a syringe holder comprising:
5 a cradle member adapted to receive a barrel of the syringe; and a pivotable catch to releasably lock the syringe in the cradle member. Preferably there is also provided a positioning device located on the cradle member to locate one end of the syringe in a predetermined location in the cradle member

According to a preferred embodiment, the syringe holder comprises an engagement portion
10 to enable simple releasable engagement with a medical injector. Preferably the engagement portion of the syringe holder comprises a locking member. The locking member of the syringe holder may comprise any suitable means of locking. Preferably it comprises a slot or a pin.

According to a further preferred embodiment, the medical injector system further
15 comprises (i) a tube adapted to be connected to syringe to conduct fluid into or out of the syringe; and (ii) a connector to connect the tube to a vessel containing medical fluid and thereby enable withdrawal of the fluid from the vessel into the syringe wherein the connector comprises a hollow spike to create an aperture through a bung in the vessel upon piercing of the bung by the spike.

20 Preferably the connector further comprises (i) a male luer portion having a locking collar; and (ii) a disengagement portion to enable permanent disengagement of the spike from the male luer portion. Preferably the disengagement portion comprises a frangible neck. Preferably the spike comprises a barbed portion to resist removal of the spike from the vessel.

25 It will be readily appreciated that the connections may comprise any convenient connection means known in the art such as bayonet, snaplock or screw connections. The spike may be broken off to leave a male luer tip on the end of an associated tube.

The combination spike, optionally a frangible (vented or sealed) spike, and male luer connector device may be permanently connected to a tube and syringe. Using this
30 combination, optimally the device can only be filled once, and thereby cannot possibly infect a multi-dose bottle of medical fluid or cross infect another patient.

If the spike connector is made as a frangible part of the connector, and is permanently attached to the tube and syringe, it is very difficult for the syringe to be refilled, and thereby cross infect the bottle or another patient. In addition, such an arrangement further reduces material costs . The syringe, spike connector means and frangible spike may be
5 supplied as one set. Preferably, the spike connector can be snapped off prior to attachment of the tube to an intravenous catheter and hence to a patient.

According to another preferred embodiment, the medical injector system further comprises a clamp between the tube and a male luer connector of the syringe, the clamp being moveable into a locking thread of the male luer connector thereby clamping the tube to the
10 male luer connector. Preferably the clamp comprises a gripping portion to increase the grip between it and the tube. The gripping portion may be of any suitable type, such as barbed rings, barbed teeth, a screw thread, serrated grip, a ridge (for example an annular ridge), a rear flange or an internal taper. In a particularly preferred embodiment the clamp is tamper evident.

15 According to a particularly preferred embodiment, the medical injector system further comprises a base member and a sensor to detect orientation of the syringe holder with respect to the base member. Preferably the sensor detects the angle between the syringe holder and base member.

According to another preferred embodiment, there is provided a switch to automatically
20 initiate or inhibit movement of the plunger in the barrel depending on its orientation. The switch may be activated by any suitable mechanism. According to one preferred embodiment, it is activated by a weight mechanism.

According to a particularly preferred embodiment, there is further provided a controller to control the plunger. Preferably at least some of the injector operation may be automated
25 by electronics or software. For example, the injector may have one or more gravity or syringe angle operated tilt switches to automatically initiate or inhibit movement of at least the syringe during operation of the injector.

According to another preferred embodiment, the system has a controller and a sensor to detect orientation of the syringe holder with respect to the base member. The sensor may
30 sense any suitable feature, but preferably it detects the angle between the syringe holder and base member.

Preferably the controller is operable to move the plunger to test patency of an intravascular catheter connected via a tube to the syringe. At present this has to be checked manually, with great care being exercised so as to avoid damaging, and possibly rupturing the vein.

Preferably a medical injector system according to this embodiment will utilize a hub,
5 plunger, syringe holder, 1 or more sensor(s) and / or syringe as herein described.

Where there is a sensor, then preferably it communicates with a controller associated with the injector system to further control the movement of the plunger. Preferably the communication enables engagement of the plunger and the hub without thereby moving the hub. According to one preferred embodiment, the communication enables releasable
10 locking of the hub to the plunger. According to another preferred embodiment, the communication causes releasable locking of the hub to the plunger. According to a still further preferred embodiment, the communication enables detection of used syringes.

According to yet another preferred embodiment, a signal is created if the sensor detects the hub at a position forward of its most retracted state. According to another preferred
15 embodiment, the communication enables detection of errors. Preferably a signal is created if the hub and plunger disengage prematurely.

According to another preferred embodiment, the communication enables movement of the plunger to either fill or expel fluid from the syringe. For example, the communication may either enable or disable movement of the plunger. This may occur for a variety of reasons,
20 or based on a variety of stimuli. For example, movement of the plunger may be disabled after use, if the syringe has not been removed, or before use if the syringe has not been engaged to a specified level.

According to another preferred embodiment, a signal is created if removal of the syringe is attempted at certain orientations of the syringe. Preferably the signal is created if removal
25 is attempted while the syringe is in a substantially vertical orientation.

According to another preferred embodiment, a signal is created indicating the syringe has not been removed. Preferably the signal is created if the syringe is not removed immediately following use.

According to a particularly preferred embodiment of the invention, there is provided
30 method of filling a syringe with medical fluid from a sealed vessel the syringe for use with

a medical injector system comprising the steps of: (i) elevating the front portion of the syringe relative to the back portion; (ii) advancing a plunger to a position within the syringe corresponding to a predetermined patient dose; (iii) controlling movement of the plunger in a sequence of forward and backward movements to expel air from the syringe and any attached tube into the vessel bottle, and draw the desired dose of fluid into the syringe.

According to a still further aspect of the invention, there is provided a method of filling a syringe with medical fluid from a sealed vessel, the syringe for use with a medical injector system as herein described, comprising the steps of: (i) elevating the front portion of the syringe relative to the back portion; (ii) advancing the plunger to a position within the syringe corresponding to a predetermined patient dose; and (iii) controlling movement of the plunger in a sequence of forward and backward movements to expel air from the syringe and any attached tube into the vessel bottle, and draw the desired dose of fluid into the syringe.

According to these methods, all outside air is excluded in order to substantially reduce the chances of introducing microbes to the fluid and patient. Furthermore, the method provides a convenient and expedient way of filling and purging both the syringe and the tube in one operation, and as well as reducing costs of materials used and speed of syringe filling as compared with traditional methods. Filling and purging of the syringe and associated extension tube may be carried out in one combined operation. According to another preferred embodiment, all elements of the fluid path are connected as one sealed system.

According to this embodiment, the combined forces of air pressure in the bottle with partial vacuum in the syringe generate a greater pressure difference between the two vessels than conventional vented systems, thereby resulting in a faster syringe filling time.

In a preferred embodiment of the method of filling, after driving of the spike connector into the bung and selection of an automatic "FILL" function on the injector, the injector then performs a sequence of controlled forward and back movements of the piston, such that all air in the syringe and tube is transferred to the bottle, and the desired dose of fluid is drawn into the syringe.

According to another preferred embodiment of the method, it further comprises the step of automatically restricting the direction of movement of the plunger depending on the

orientation of the syringe. Preferably the plunger may move either forward or backward when oriented with its front portion elevated with respect to its back portion and only in the forward direction when oriented with the back portion elevated with respect to its front portion. This reduced the chance of an air bubble being injected into a patient by ensuring
5 that air bubbles will be at the back of the syringe. Preferably this step may be enabled by a tilt switch or sensor so that the syringe is inclined with the front portion elevated when expelling air and filling so to minimise trapping of air in the syringe.

According to another aspect of the invention there is provided a method of injecting a patient using a medical injector system as herein described comprising the steps of (i)
10 engaging the plunger with the hub, (ii) driving the hub along the syringe barrel; and (ii) expelling fluid from the syringe into a patient.

According to a further aspect of the invention, there is provided a method for engaging a syringe holder as herein described with a medical injector according to claim [ind], comprising the steps of: (i) aligning the engaging portion of the syringe holder with a
15 complimentary portion on the medical injector; and (ii) engaging the syringe holder with the medical injector.

According to one preferred embodiment, there is the further step of detecting a level of engagement between the syringe holder and the medical injector system.

According to a still further aspect of the invention, there is provided a method for
20 disengaging a syringe holder as herein described from a medical injector as herein described comprising the steps of: (i) disengaging the engaging portion of the syringe holder from the medical injector; and (ii) removing the syringe holder from the medical injector.

Preferably there is the further step of detecting a level of disengagement between the
25 syringe holder and the medical injector system.

According to a further aspect of the invention, there is provided a method for loading a syringe into a syringe holder associated with a medical injector system as herein described, comprising the steps of: (i) inserting the syringe barrel in the cradle member such that the catch is displaced; and (ii) allowing the catch mechanism to return into its biased position
30 to engage the syringe and thereby retain the syringe in the cradle member.

According to a still further aspect of the invention there is provided a method for removing a syringe from a syringe holder associated with a medical injector system as herein described comprising the steps of: (i) releasing the catch to unlock the syringe; and (ii) withdrawing the syringe from the cradle member.

- 5 According to a further aspect of the invention, there is provided a method for loading a syringe into a syringe holder of a medical injector system as herein described comprising the steps of: (i) inserting the syringe barrel in a cradle of the syringe holder; and (ii) sensing the presence of the syringe in the holder with a sensing member associated with the sensing system.
- 10 According to a further aspect of the invention, there is provided a method for removing a syringe from a syringe holder of a medical injector system as herein described comprising the steps of: (i) withdrawing the syringe from the cradle member; and (ii) sensing the absence of a syringe in the holder with a sensing member associated with the sensing system. Preferably there is the further step of automatically retracting the plunger after
- 15 withdrawal of the syringe. Preferably there is a still further step of restricting retraction of the plunger until the syringe has been withdrawn. According to one preferred embodiment, there is a further step of prompting retraction of the plunger after the syringe has been withdrawn.

- According to another aspect of the invention, there is provided a method of connecting a syringe hub to a plunger using a medical injector system as herein described comprising
- 20 the steps of: (i) introducing the plunger into a syringe barrel within which the hub is slidably engaged and engaging the plunger with the inner surface of the hub; and (ii) activating the plunger such that a retention member engages the engaging portion of the hub. Preferably there is the further step of detecting a level of engagement between the
- 25 plunger and the hub.

- According to a further aspect of the invention, there is provided a method for modifying a medical injector system comprising a syringe holder, comprising the steps of: (i) replacing the syringe holder with a syringe holder as herein described; and (ii) attaching a plunger as herein described.
- 30 According to another aspect of the invention, there is provided a method for modifying a medical injector system comprising a syringe holder, comprising the steps of: (i) replacing

the syringe holder with a syringe holder as herein described; and (ii) attaching a plunger as herein described.

According to a further aspect of the invention, there is provided a method for modifying a medical injector system comprising the steps of: (i) replacing the syringe holder with a
5 syringe holder as herein described; and (ii) attaching a plunger as herein described.

According to another aspect of the invention, there is provided a method for modifying a medical injector system comprising the step of adding a sensing system as herein described.

Brief Description of the drawings

- 10 Figure 1 shows a prior-art injector with a syringe loaded;
- Figure 2a shows various components of the syringe as used in the present invention;
- Figure 2b shows an assembled syringe;
- Figure 2c shows the assembled syringe of Figure 2b in conjunction with a plunger;
- Figure 3a shows oblique side views of the hub;
- 15 Figure 3b shows a side view of the hub;
- Figure 3c shows a cross sectional view of the assembled hub and seal;
- Figure 3d shows a front view of the hub;
- Figure 3e shows a rear view of the hub;
- Figure 4a shows alternative conformations of the engaging portion of the hub, in the
20 form of grooves;
- Figure 4b shows a cross section of the hub and engaging portion;
- Figure 4c shows a cross section of the hub and engaging portion, having a conventional seal, with an extended leading edge;
- Figure 4d shows a cross section of the hub and engaging portion, having a seal integral
25 to the hub;

- Figure 4e shows a cross section of the hub and engaging portion, having an o-ring seal;
- Figure 4f shows further alternative conformations of the engaging portion of the hub;
- Figure 5 shows example dimensions of the hub;
- 5 Figure 6 shows a cross-section of the plunger engaging the hub;
- Figure 7 shows a cross sectional side view of one possible embodiment of the plunger/hub interlocking arrangement;
- Figure 8 shows a front cross-section along the line A - A of Figure 7;
- Figure 9 shows an alternative arrangement of Figure 8;
- 10 Figure 10 shows an alternative example of the plunger/hub interlocking arrangement;
- Figure 11 shows a front cross-section along the line A - A of Figure 10;
- Figure 12 shows an alternative arrangement of Figure 11;
- Figure 13 shows an alternative arrangement for the plunger/hub interlocking arrangement;
- 15 Figure 14 shows a front cross-section along the line A - A of Figure 13;
- Figure 15 shows yet another alternative of the plunger/hub interlocking arrangement;
- Figure 16 shows a front cross-section along the line A - A of Figure 15 showing the cam in detail;
- Figure 17 shows yet another alternative example of the plunger / hub interlocking arrangement, having a ring actuated hub locking mechanism;
- 20 Figure 18a shows a side view of the syringe holder with catch;
- Figure 18b shows the syringe holder and catch of Figure 18a with the syringe and hub located in the syringe holder;
- Figure 18c shows a side oblique view of the syringe holder and catch of Figure 18a;

- Figure 18d shows a side oblique view of the syringe holder, catch and syringe of Figure 18b;
- Figure 18e shows a side oblique view of a syringe holder, catch and syringe according to the present invention;
- 5 Figure 19 shows a cross section side view of the syringe holder/syringe combination within the sleeve of the injector, with the syringe retained by a catch;
- Figure 20 shows a cross-section along the line A - A of Figure 19;
- Figure 21 shows a cross-section along the line B - B of Figure 19;
- 10 Figure 22a shows a cross section side view of the syringe holder/syringe combination within the sleeve of the injector, with the syringe retained by a catch depicting the illumination member;
- Figure 22b shows the arrangement of Figure 19 with a self-ejecting mechanism;
- Figure 23a shows a plunger adapted to be a syringe hand filler and associated holder;
- Figure 23b shows a syringe and syringe holder comprising a concave syringe front flange and corresponding dovetail catch;
- 15 Figure 23c shows a perspective view of a syringe with a concave front flange;
- Figure 23d shows a cross-sectional view of a syringe with a concave front flange;
- Figure 23e shows a cross-sectional view of a dovetail catch according to the present invention;
- 20 Figures 23f demonstrates in cross-section, various alternative arrangements of catches according to the present invention;
- Figure 24 shows the connection and orientation of certain key elements in the system, as oriented during the filling sequence;
- Figure 25 shows an example of a Barbed Spike for tapping the bung of a medical fluid bottle;
- 25

- Figure 26 shows various views of an example of a combination male luer connector and frangible spike;
- Figure 26a is an oblique view of combination Luer connector with frangible spike, locking collar, and tube, before assembly;
- 5 Figure 26b is a longitudinal axial cross-section view of combination Luer connector with frangible spike, and locking collar, after assembly;
- Figure 26c shows a combination Luer connector with frangible spike, locking collar, and tube, after assembly and bonding;
- Figure 26d is a combination Luer connector with frangible spike and locking collar,
10 shown after the spike has been “snapped off” at the frangible neck;
- Figure 27 shows an example of a male Luer Connector with barbed frangible spike, and locking collar, as follows:
- Figure 27a shows a longitudinal axial cross-section view of a Luer Connector with barbed frangible spike, locking collar, and bonded tube;
- 15 Figure 27b shows an example of a Luer Connector with barbed frangible spike and locking collar, after assembly and bonding; and
- Figure 27c shows a shorter example of a Luer Connector with barbed frangible spike, locking collar, and bonded tube;
- Figure 28 shows a combination Luer Connector with frangible spike, permanently
20 bonded to the associated Extension Tube and Syringe to form a non re-usable set for injecting patients;
- Figure 29 illustrates a typical syringe male Luer lock connector;
- Figure 29a shows an outer overall view of the luer lock of Figure 30;
- Figure 29b Figure shows a longitudinal axial cross-sectional view of a typical syringe
25 luer lock connector;
- Figure 30 illustrates a longitudinal axial cross-sectional view of an ordinary soft plastic tube pushed over the tip of a typical luer.;

- Figure 31 demonstrates various views of the basic or Plain form of a clamp according to the present invention;
- Figure 31a demonstrates a side view of the Plain clamp;
- Figure 31b demonstrates an oblique view of the Plain clamp;
- 5 Figure 31c depicts the Plain Clamp in longitudinal axial cross-section.;
- Figure 31d depicts a longitudinal axial cross-sectional view of a soft plastic tube pushed over the tip of a luer, and the plain clamp pressed into the female locking thread of a luer locking syringe;
- Figure 32 depicts a clamp with barbed rings;
- 10 Figure 32a depicts an oblique outer view of a clamp having annular barbed rings added to the outer surface;
- Figure 32b depicts a longitudinal axial cross-sectional view of a clamp having annular barbed rings added to the outer surface;
- Figure 32c depicts a longitudinal axial cross-sectional view of a barbed clamp pressed
15 into the female locking thread of a luer locking syringe, and clamping a tube onto the associated male luer tip;
- Figure 33 depicts a clamp with male threads;
- Figure 33a depicts a plain clamp with male threads;
- Figure 33b depicts a plain clamp having male outer threads, with the addition of
20 serrated grip to the rear end of the clamp;
- Figure 33c depicts a longitudinal axial cross-sectional view of a plain clamp having male outer threads added to the outer surface;
- Figure 33d depicts a longitudinal axial cross-sectional view of a clamp having male
25 outer threads, screwed into the female locking thread of a luer locking syringe, and clamping a tube onto the associated male luer tip;

- Figure 33e depicts a longitudinal axial cross-sectional view of a clamp having male outer threads, with the addition of an annular ridge added to the inside surface of the clamp;
- 5 Figure 33f depicts a longitudinal axial cross-sectional view of a clamp having male outer threads plus an annular internal ridge, screwed into the female locking thread of a luer locking syringe, and clamping a tube onto the associated male luer tip;
- Figures 34 & 35 illustrate flanges added to the rear end of clamps;
- 10 Figure 34a illustrates a side view of a Threaded Clamp with a plain flange added to the rear end of the clamp;
- Figure 34b illustrates a rear view of a Threaded Clamp with a plain flange added to the rear end of the clamp;
- Figure 35a illustrates a side view of a Tamperproof Threaded Clamp having barbed teeth added to the outer perimeter of the flange;
- 15 Figure 35b illustrates a rear view of a Tamperproof Threaded Clamp having barbed teeth added to the outer perimeter of the flange;
- Figure 36 illustrates a side perspective view of a syringe holder with an engagement portion to enable releasable engagement with a medical injector and sensing system to detect the presence of the syringe;
- 20 Figure 37a illustrates an exploded perspective view of a syringe holder with a bayonet attachment, loaded syringe and sensing system to detect the presence of a syringe;
- Figure 37b illustrates a cross-sectional view of the holder and syringe of Figure 37a;
- Figure 37c illustrates a syringe flag for use with the syringe sensing system;
- 25 Figure 37d illustrates a cross sectional view of the injector nose with holder lock post;
- Figure 38a illustrates a longitudinal cross-sectional view of a syringe holder with a bayonet attachment, loaded syringe and sensing system to detect the presence of a syringe;

- Figure 38b illustrates a lateral cross sectional view of the syringe holder and syringe of Figure 38a through the line MM;
- Figure 38c illustrates a lateral cross sectional view of the syringe holder and syringe of Figure 38a through the line LL;
- 5 Figure 38d illustrates a lateral cross sectional view of the syringe holder and syringe of Figure 38a through the line KK;
- Figure 38e illustrates a syringe flag for use with the syringe sensing system;
- Figure 39a illustrates a cross sectional view of a syringe in a syringe holder demonstrating a particularly preferred embodiment of the engagement mechanism between the hub and plunger during movement of the plunger to expel fluid from the syringe;
- 10 Figure 39b illustrates the syringe and syringe holder of Figure 39a during movement of the plunger to draw fluid into the syringe;
- Figure 40 illustrates a longitudinal cross sectional view of a plunger and hub demonstrating a preferred embodiment of the sensor to detect engagement between the hub and plunger;
- 15 Figure 41 illustrates an injector with tilt switches in the injecting (down) position;
- Figure 42 illustrates an injector with tilt switches in the filing (up) position;

Description of preferred embodiments

- 20 A typical injector system used for similar applications as the present invention includes an automatic injector device 100. The injector will normally have a data entry pad 110 together with a display 120 for entering data and viewing data respectively. The type of data that may be entered into the system includes injecting rates and volumes. The system according to the prior art includes a pressure jacket or sleeve 140 which is connected to
- 25 injector 100 for retaining an appropriate syringe 300. Tube 400 connects syringe 300 to the patient (not shown). The prior-art arrangement of the injector as shown in Figure 1 suffers from a number of disadvantages. Firstly, to install syringe 300 into injector 100, sleeve 140 must first be removed or opened to allow syringe 300 to be rear- or breech-loaded into the sleeve 140 and fixed therein by reattaching or closing sleeve 140. In some

cases, sleeve 140 is completely closed, like that shown in Figure 1, requiring that tube 400 be attached after loading and removed before unloading the syringe 300. This increases the amount of time required to load the syringe, and increases the risks of spillage of contaminated blood. These disadvantages are addressed by the system of the present invention, which allows the syringe 300 to be loaded into the injector 100 directly from the front and does not require sleeve 200 to be removed, loaded and re-inserted into injector 100.

To allow syringe 300 to be inserted easily from the front, the syringe itself may be flangeless. That is, the outer cylindrical surface of the syringe may be free of any interfering projections which normally exist on syringes.

A syringe in accordance with the present invention is shown in Figure 2a wherein there is shown the barrel of the syringe 300, into which are inserted a hub 310 and corresponding seal 320. Upon assembly of hub 310 and barrel 300, the syringe appears as shown in Figure 2b. The hub and seal can be manufactured as one component [illustrated in Fig.4d]. For the preferred embodiment the hub is made from semi-rigid plastic, whilst the seal is made from elastomer. In practice, manufacturers of the syringe could sell the syringe barrel either empty, or pre-filled with the required amount of medical fluid to be injected into the patient, which is retained inside the barrel by the hub and seal combination.

To inject the drug contained within the syringe, a plunger 130, which is operatively connected to the injector 100, engages the inner surface of the hub 310 and it is actuated by the injector 100 in accordance with the required controlled motion. As plunger 130 is driven into syringe barrel 300, this causes hub 310 and seal 320 to be driven relatively towards the other end of barrel 300, thereby injecting the drug through tube 400 into the patient (not shown). The hub according to the present invention may be made of any suitable semi-rigid plastic such as polypropylene or styrene, whilst the seal could be made from an elastomeric substance such as Santoprene, Kraton, Improflex, Kraiburg. etc.

The hub 310 is shown from various angles in Figure 3. In particular, annular groove 311 is shown on the inside surface of hub 310. The cross-section of the groove may take on any appropriate shape as shown in Figure 4a including, semi-circular, squared and triangular cross-sections. In addition, Figures 4c shows a hub assembled with a seal 320 having an extended leading edge on the seal lip to improve sealing under pressure. Figure 4d shows

a hub and seal combined in one piece which provides the benefits of reduced manufacturing costs. Other advantages of this arrangement are also apparent such as (1) increased lubricity if a low friction material such as polypropylene is used, (2) elimination of silicone or other lubricants, (3) reduction of particles in syringe; and (4) reduced /
5 eliminated assembly costs. The purpose of this groove will be described in more detail below. Figure 4e further depicts a hub having an annular seal 312 seen in cross section.

The dimensions of the hub will obviously be made in accordance with the particular syringe being used. By way of example, it is envisaged that they will typically be of the order of the dimensions shown in Figure 5.

10 The tip of injector plunger 130 is formed so as to effectively engage with the inner surface of hub 310 as clearly shown in Figure 6. Annular groove 311 is also clearly seen as defining a space between the wall of the hub 310 and the surface of the tip of injector plunger 130. This engagement between plunger 130 and hub 310 is such as to provide a form fit so that the force actuated by injector plunger 130 is efficiently imparted to hub
15 310, causing the hub and associated seal 320 (not shown in Figure 6) to travel forward along the inner surface of syringe 300, and thereby expel the contents of the syringe.

It is envisaged that injector plunger 130 will be useful for emptying a pre-filled syringe. However, empty new syringes are often filled just prior to use within such injectors, which requires the hub and seal to be retracted by plunger 130. It will be seen that by itself,
20 plunger 130 does not grip or retain hub 310. Therefore another mechanism is required to allow plunger 130 to effectively grip hub 310 and enable it to withdraw the hub and seal from the syringe barrel. Groove 311 provides such a mechanism.

As can be seen in Figure 7, upon retraction of the plunger, pins 142 protrude from plunger 130 at the location of groove or recess 311. Pins 142, filling groove or recess 311, act as
25 retention members allowing hub 310 to be withdrawn from the syringe barrel 300 as injector plunger 130 is withdrawn. The mechanism by which pins 142 are caused to enter groove or recess 311 may take on many forms as now discussed in further detail in Figures 7 to 16.

In one embodiment as shown in Figure 7, plunger 130 may include actuating rod 140 with
30 a cam element 141 projecting from a nose end of actuating rod 140. Cam element 141 is an oval-shaped rod, which upon insertion of plunger 130 into syringe barrel 300, lies in a

horizontal plane. Pins 142 rest against the outer surface of cam element 141 and are biased towards cam element 141 via springs 143. In this position, the outer ends of pins 142 lie within or below the surface of plunger 130. Once the plunger/hub/seal arrangement has reached the end of syringe barrel 300, and is required to be retracted from the barrel, 5 actuating rod 140 may be rotated about its axis, such that cam element 141 now lies in a vertical plane as shown in Figure 8. As cam element 141 rotates, pins 142, which are biased against the surface of cam element 141, are caused to be pushed out towards the surface of plunger 130 such that their outer ends protrude from plunger 130 and are received in groove or recess 311 as shown in Figure 7. In this position, hub 310 is retained 10 by plunger 130 and is able to be withdrawn from syringe barrel 300. As discussed above, this mechanism may take on many forms, a further one of which is shown in Figure 9. In this case, cam element 141 may have a square cross-section which allows the four pins 142 to be extended from plunger 130 to be received in groove or recess 311. The heads of pins 142 are biased against the four sides of cam element 141 and upon rotation of cam element 15 of 141, are caused to be biased against the four corners of cam element 141, resulting in pins 142 protruding from the surface of plunger 130.

In another embodiment of a mechanism for actuating pins 142 shown in Figures 10 to 12, cam element 141 is replaced by a cone element 144. In this embodiment, pins 142 are biased against the outer surface of cone element 144 by springs 143 as in the previous 20 embodiment. In use, plunger 130 is inserted into syringe barrel 300 and hub 310, whilst actuating rod 140 is pressed as far as possible against the forward surface 131 of plunger element 130. In this position, pins 142 rest against the narrowest portion of cone element 144 and are biased away from the outer surface of plunger 130 by springs 143. Before or upon retraction of plunger 130, actuating rod 140 is pulled away from surface 131 causing 25 pins 142 to slide along cone element 144 up the cone surface. This causes pins 142 to be pushed out and to protrude from the outer surface of plunger 130 to be received in groove or recess 311. Hub 310 is thereby retained by plunger 130 and able to be moved along the syringe barrel 300. This arrangement also allows for four pins to be used to be received in groove or recess 311 as shown in Figure 12. The cone arrangement of Figures 10-12 may 30 also be used in a "gravity operated" locking mechanism whereby plunger 130 only retains hub 310 when the syringe assumes a particular orientation. Such an arrangement (as shown in Figures 13 and 14) is particularly useful when it is desired to prevent re-use of a

syringe between patients. This is desirable to reduce the risks of cross-patient infection or contamination.

It will be appreciated that it is advisable to tilt the injector upward during syringe filling in order to ensure that air is kept at the syringe outlet for subsequent removal prior to
5 injection. Additionally, it is advisable to tilt the injector downward during injection (to keep any remaining air in the syringe by the hub so that any air will remain in the tubing between the syringe and the patient after the injection, and therefore not enter the patient.

Generally, new syringes are supplied with the hub and seal arrangement placed in a fully retracted position, ie near the back of syringe barrel 300. It is also customary to retract the
10 plunger following each use. In one embodiment, with the injection unit 100 oriented down, the syringe is loaded through the front end of the cylindrical sleeve in the injector unit, which aligns the syringe with the plunger. As a consequence, hub 310 engages plunger 130. It should be noted that if a used syringe had been loaded, the hub would not engage the fully retracted plunger (i.e., because the hub would not be in the fully retracted position
15 within the syringe barrel). To fill the syringe, the injector with the syringe loaded therein is then tilted vertically. As the injector unit is tilted vertically weight rod element 145 drops down within a cylindrical cavity 132 in plunger 130 as shown in Figure 13. As weight rod element 145 drops, cone element 144 causes pins 142 to be pushed out to protrude from the outer surface of plunger 130 to be received in groove or recess 311 of
20 hub 310. Thus, hub 310 is retained by plunger 130. Upon tilting up, plunger 130 is able (through an automatic tilt switch and controls) to push hub 310 and associated seal 320 (not shown) towards the top end of syringe barrel 300 until the plunger cannot advance any further and seal 320 rests up against the front end of syringe barrel 300, expelling the unwanted air.

25 Upon actuating the plunger in the reverse direction, hub 310 and seal 320 are retracted and the syringe is able to be filled. To inject the contents of the syringe into the patient, the injector unit is returned to a downward position and plunger 130 is once again advanced along syringe barrel 300, expelling the contents of the syringe. As the injector assembly assumes a downward orientation, weight rod element 145 returns to a forward-most
30 position within cavity 132. This causes pins 142 to be retracted below the outer surface of plunger 130 due to springs 143 and due to the fact that the heads of pins 142 are now allowed to rest against the narrow portion of cone element 144. Upon completion of the

injection procedure, plunger 130 is automatically retracted from syringe barrel 300 and, because pin elements 142 have been retracted into plunger 130, hub 310 is no longer retained by the plunger and therefore remains at the front-most portion of syringe barrel 300. Accordingly, the used syringe (whether just used, or later reloaded) cannot be reused
5 because given that hub 310 has been advanced (at least partially) along the syringe barrel 300, the hub will not be engaged with the fully retracted plunger 130, and cannot be retained when the injector is tilted up.

If the injector unit was raised to assume a vertical position again, weight rod element 145 drops down due to gravity, causing pins 142 to extend beyond the top surface of plunger
10 130. If plunger 130 were advanced into the barrel 300, it will not be able to proceed past the back end of hub 310 due to the protrusion of the pins. This will alert the unit operator that the syringe has been used and prompt them to obtain an unused syringe.

Yet a further possible implementation of the locking mechanism involves the use of cam element 154 connected to an actuating rod 133 which is contained within the body of
15 plunger 130. This arrangement is shown in Figures 15 and 16. During the advancement of plunger 130/hub 310/seal 320 combination into the barrel 300 of the syringe, actuating rod 133 is orientated such that cam element 134 is positioned with its nose pointed downwards from the point of view of Figures 15 & 16, such that no part of cam element 134 protrudes from plunger 130. Once hub 310 with seal 320 (not shown in figures 15 or 16) is then
20 required to be retracted, actuating rod 133 is rotated in the direction of the curved arrows such that the nose of cam element 134 protrudes from the surface of plunger 130 and is received in groove or recess 311. In this manner, hub 310 and connected seal 320 are retained by plunger 130 and may be retracted within the syringe barrel upon retraction of plunger 130.

25 It will also be appreciated that pin elements 142 (Figures 7 to 14) need not be individual pins but may take the form of a unitary ring within plunger 130 which may lie flush with or below the surface of plunger 130 during the advancing stage and which may be caused to expand to protrude from the surface of plunger 130 to be received in groove or recess 311.

Such an arrangement is shown in Figure 17, in which plunger 130 is divided into two
30 sections - a main body portion 139 and a nose portion 136. Connecting these two portions is an actuating rod 135, a front end of which is embedded in nose portion 136. By pushing

actuating rod 135 forward, nose portion 136 is caused to be longitudinally displaced by a small amount, forming gap 137 between main body portion 139 and nose portion 136. The radial ends of gap 137 are chamfered, creating void 138, the size of which is dependent on the size of gap 137. Within void 138, lies an expandable ring 800. This may be a rubber
5 o-ring, a metal circlip, or any other suitable ring element. Ring 800 is biased towards its centre, such that it will tend to lie as deep as possible within void 138, and below the surface of plunger 130. This will be the position assumed when plunger 130 is moving forward along the syringe.

To retract hub 310, actuating rod 135 is moved backwards to cause gap 137 to close, in
10 turn causing void 138 to become smaller. This in turn pushes ring 800 radially outwards, to protrude from plunger 130, and to be received in groove or recess 311, thereby retaining hub 310 to plunger 130.

It will be understood that groove or recess 311 need not in fact encompass the full circumference of the inner surface of hub 310, but may take the form of individual recesses
15 or depressions within the surface of hub 310 to receive individual pins from plunger 130. It will be understood that if rod 135 were the driving member of the injector, and plunger body 139 were restrained by a friction ring system such as that described in Figs 39a and 39b, the hub retention function described above will operate automatically.

The loading and retention of syringe barrel 300 inside injector unit 100 will now be
20 described with reference to Figures 18a-e to 21. Figures 18a to 18d show various views of a syringe cradle member in the embodiment wherein the cradle member is a sleeve 200 and associated catch 500. Figure 18e depicts the embodiment wherein the cradle member is a cradle 205 containing syringe barrel 300.

The left-most (rear) end of sleeve 200 (from the view of the depictions) is inserted into a
25 receiving opening in the injection unit, while syringe barrel 300 is slipped rear first into sleeve 200 via the oblique opening appearing on the right hand side of sleeve 200 as seen from the figures. Figures 18b and d show various views of the embodiment wherein the cradle member is a sleeve 200 containing syringe barrel 300. Also visible are hub 310 and connected seal 320 which are positioned at the base end of syringe 300 as described
30 previously. Catch 500 is pivotally connected to sleeve 200 as can be seen in Figures 19, 20 and 21. Syringe holder 200 is engaged in nose 10 of the injector (not shown). The

connection between catch 500 and holder 200 is via catch hinges 510. Spring 540 biases one end of catch 500 away from the body of sleeve 200 such that syringe catch 520 is biased upwards and through sleeve aperture 530 as seen in Figure 19. Upon insertion of syringe barrel 300 into sleeve 200, syringe catch 520 is displaced downwards by a downward force caused by the syringe sliding across the sloped top surface of syringe catch 520 (actuated by a human operator). Once syringe barrel 300 has been fully inserted into sleeve 200 (determined by syringe stop ring 210), spring catch 520 snaps back to assume its steady state position to engage a front portion 330 of syringe barrel 300, thereby retaining it within sleeve 200. This retention is strong enough to withstand the pressure experienced by the syringe upon actuation of the injector forcing plunger 130 into the barrel 300 to expel the contents of the syringe. In fact, the upright front edge 521 of catch 520 is angled so that it lies parallel to the front edge of sleeve aperture 530, which is itself similarly angled. This angle is chosen carefully to be greater than 90 degrees to the moment of force exerted by flange 330 on forward edge of aperture 530. In this way, the engagement forms a wedge or "dove-tail", which prevents catch 520 from being released when the syringe is forced forward by the plunger, thereby providing a highly secure retention means.

Furthermore, syringe sleeve 200 is close-fitting to the inserted syringe barrel 300. This helps to support the syringe against expansion under the high pressures caused in injectors, thereby enabling a thinner walled, lower cost syringe. Sleeve 200 is also preferably transparent, to allow an unobstructed view of the contents of the syringe (e.g., to determine if air is present in the syringe), which itself is transparent.

As discussed previously, this arrangement allows the syringe to be loaded into the injector unit in a single action by simply sliding it into a receiving sleeve from the front and without having to remove any part of the injecting unit. Further, the syringe and the hub need not be oriented in a particular manner. This saves a great deal of time and effort in syringe assembly and everyday use of the injector, and results in a simpler construction of the injector.

Figure 22a demonstrates another preferred embodiment whereby there is an illumination member in the form of Light emitting diodes (LEDs) 4200 which are placed at the exposed rear (left-most) end of syringe sleeve 200 so that some of the light is received and transmitted along the walls of the sleeve. As with any thin, dense, transparent material ,

most of the received light is internally reflected longitudinally, as well as laterally, producing a diffused glow at the front end of the sleeve as depicted by arrows 4250. The beveled front end of the sleeve 4255 is preferably frosted (eg sanded) to achieve maximum diffusion, and is visible from a wide angle. Any suitable light source may be used, but they are preferably focused or reflected so that most of their output is projected towards the sleeve. Thus, in the embodiment depicted, they are LEDs.

The illumination sources may be various colours, and / or pulsed to provide many attractive effects, and may be used to remind the operator, for example, to remove the syringe.

It should be noted that the patient's blood may sometimes find its way into tube 400 and syringe 300 by virtue of the fact that, on occasion, while connected to the patient, the hub is retracted to draw blood back through tube 400 and into the syringe, for example to verify that the needle has properly entered the patient's vein. Since the syringe can be loaded from the front, tube 400 (as depicted in the Figure 1 in relation to the prior art), may be permanently fixed to the syringe, and need not be connected and disconnected after use. This reduces the risk of spilling contaminated blood.

To further increase the efficiency of the system, syringe stop ring 210 may consist of 2 parts, separated by a spring element 220, as shown in Figure 22b. The first part is a fixed part 210a which is essentially a portion of stop ring 210 in Figure 18 and is fixed to syringe sleeve 200. The second part is a sliding ring 210b, which is able to slide over the inner surface of sleeve 200. Coil Spring element 220 biases sliding ring 210b away from fixed ring 210a and towards the front end of sleeve 200. When the syringe 300 is loaded into sleeve 200, its rear rim will engage slide ring 210b and force it towards fixed ring 210a, compressing spring element 220 there between, until spring catch 520 snaps back to retain syringe 300 as described above. In this state, syringe 300 is biased against catch 520 by the force of spring element 220 acting on sliding ring 210b. Accordingly, when syringe catch 520 is disengaged from syringe 300 (by pushing on syringe catch release button 550), syringe 300 is automatically partially ejected from sleeve 200 to facilitate removal thereof from the injector.

Some injector users prefer to manually fill syringes without the use of an injector. This ability is also of great benefit when users wish to pre-fill syringes, particularly when the injector is in constant use.

On the occasions where a syringe is desired to be manually filled, the present invention also provides for easy filling of the syringe. This is accomplished by way of a hand filler 700 as shown in Figure 23a. This device is effectively a hand-held version of the plunger 130 described in detail above, and works in a similar manner. In use, the hub 310 and seal 320 could be located anywhere along the syringe. To fill the syringe, the hub/seal must be drawn back towards the rear of the syringe. To do this, hand plunger 700 is introduced into the syringe barrel 300, and pushed into the hollow of hub 310. In this position, pins 750 within the head of the hand filler do not protrude beyond the surface of the hand plunger 700. This is because cone element 730, inside the hand filler, is biased forward by spring elements 740, causing pins 750 to rest against the narrowest portion of cone element 730. Upon retraction by hand (with the fingers 610 of the operator engaging the handle 710 of the plunger), cone element 730 is pulled back with the head of hand plunger 700, forcing pins 750 outwards to be received in groove or recess 311, thereby engaging hub 310 and seal 320. Thus engaged, the hub and seal are drawn back through syringe 300 with the hand plunger 700, at the same time drawing in liquid through hole 340 and filling the syringe. When the hub 310 and seal 320 have reached the back of the syringe, hand plunger 700 is disengaged from hub 310 by reducing backward force on the plunger, allowing cone element 730 to move forward under the force of spring element 740, and allowing pins 750 to withdraw from recess or groove 311 as previously described. The filled syringe is then ready to be loaded into the injector 100 as described above. It should be noted that no part of the device can, at any stage touch the inner bore of the syringe, which could contaminate the sterility of the syringe. It should also be noted that the mechanism retaining the hub to the plunger can take many forms, including those described in Figures 7 to 17.

In another embodiment, the filled syringe may be left connected with the hand filler, and the combination may be connected at the neck 735 to the front end of a suitably modified injector. In this application, the hand filler becomes a syringe holder and pressure sleeve. The complete hand filler device is used to firstly fill the syringe, then the filler device (with

syringe) is placed into the injector. The injector pushes on the rear end 710 to expel fluid from the syringe.

Where the hand filler device illustrated is provided only for filling (in association with an injector made for injecting the syringe), then as long as all syringes are fully expelled (as is the convention), then if the length of the plunger 700 were shortened by only a few millimetres, it could not fill a used (fully expelled) syringe because it can not reach the hub.

In a further embodiment, the contents of syringe 300 can be expelled by hand force on plunger knob 710 (i.e., an injector syringe such as 300 could be used as a more conventional hand-held syringe).

As with most injector syringes, syringes as used in the present invention are preferably supplied with the hub/seal in the fully retracted position.

The various mechanisms for retaining the hub to the plunger of the present invention are preferably arranged such that they can be actuated whilst the plunger is in the fully retracted position, and thereby preferably engage, retain, and fill a new syringe. However, the invention contemplates that the plunger can be arranged to engage the hub at any suitable location within the syringe.

Following use, the hub and seal of a used (or partially used) syringe will typically be left somewhere forward of the fully retracted position, and hence the devices of the present invention usually do not engage, retain, fill or operate a used syringe, thereby eliminating, or drastically reducing, instances of cross-patient contamination. However, the invention broadly contemplates arrangements wherein the hub can be left at any position within the syringe.

It will readily be appreciated that there are a number of possible designs for the catch for retaining the syringe within the cradle member /sleeve. Figures 23b to 23e illustrate a syringe 300 and syringe holder 200, catch 500 and catch member 520. The inner edge 526 of the catch 520 is of complementary shape to a concave front flange on the syringe 300. Figure 23f shows three embodiments of the interface between the inner edge of the catch 520 and the front of the syringe 300.

The preferred embodiment of an additional embodiment of the invention comprises the essential elements illustrated and oriented as shown in Figure 24. An extension tube 1010 is firstly fitted to the tip 1012 of an injector syringe 1014. The syringe 1014 is then fitted to an injector (or syringe pump) 1016. The system operator (not shown) then programs the desired patient injection volume on the injector control panel (not shown), and then the operator tilts the combined injector 16 and syringe 1014 unit upwards as illustrated in Figure 24, at which point a position or angle sensing tilt switch in the injector preferably causes the piston 1032 of the syringe 1014 to advance automatically by the injector to the desired volume. It will be appreciated by those familiar with the art that such programming and automatic control of the injector is quite known, although not in response to the tilting operation, or means of triggering. Of course, the operator could also initiate some or all of these actions. As the combined injector 1016 and syringe 1014 unit is tilted upwards, any subsequent fluid 1028 from bottle 1026 will fall to the bottom of syringe 1014, and air 1030 in the syringe 1014 will rise to the syringe tip 1012, and be expelled through tube 1010 when the piston is advanced. The free end of tube 1010 is then connected to the socket end 1018 of a special non-vented spike 1020 which is shown in Figure 24, and in more detail in Figure 25. The sharp end 1022 of spike 1020 is then driven into the soft rubber bung 1024 of the fluid bottle 1026. The sharp tip 1022 of spike 1020 pierces the bung 1024 of the bottle 1026, creating a path from the bottle contents 1028 through the spike 1020 and tube 1010 to the syringe. It should be noted that at this point the system is sealed from outside air, and pressure in the system will be neutral. It should also be noted that spike 1020 has a barbed neck 1021 as shown in Figure 25 to ensure it will not be forced out of the bung 1024 when the system is later pressurised. The bottle 1026 is then mounted or hung inverted (as illustrated in Figure 24) so that fluid 1028 can be drawn out through the spike 1020 and tube 1010 etc.

The "FILL" button (not shown) is now selected on the injector 1016 by the operator, and preferably performs the following sequence automatically:

The syringe piston 1032 is driven fully forward to the tip 1012 of the syringe 1014, compressing the air 1030 in the syringe, tube, and bottle. Much of the sterile air 1030 in the syringe and tube 1010 will be driven into the bottle 1026, and rise to the air space 1034 in bottle 1026. It will be appreciated by those familiar with the art that such air 1030 will be sterile as long as the syringe 1012 was manufactured and sterilised with the hub 1032

fully retracted (i.e. filled with air) as illustrated in Fig 2b. Without delay, the piston 1032 is then automatically retracted to slightly over (eg 130%) the programmed volume, and fluid 1028 is transferred quickly from the bottle 1026 via spike 1020 and tube 1010 into the syringe 1014, aided by both air pressure 1034 in the bottle 1026, plus a partial vacuum in
5 the syringe due to retraction of piston 1032. Following a short delay to allow the pressure to equalise and fluid to fully transfer, the syringe 1014 is filled to more than the programmed fluid volume, plus some residual air. The piston 1014 is then immediately and automatically advanced back to the desired programmed volume, purging any residual air and surplus fluid back to the bottle 1026, leaving the syringe 1014 entirely filled with the
10 programmed volume of fluid, with no air in either the syringe 1014, or tube 1010.

At this stage the "FILL" sequence is complete, and it is important to note that the system has neutral pressure (because the piston has been returned back to the position at which the system was sealed) so that when the tube is disconnected from the bottle (or the spike is removed), the system neither sucks air, nor drips fluid.

15 The bottle 1026 is now righted, and the tube 1010 is disconnected or detached from the spike connector 1018, and may now be connected to the patient, ready for injection.

It will be appreciated by those familiar with the art that the following facts and arrangements are normal procedure in this field, and may not be well illustrated or described in this document, however are important to the implementation and operation of
20 the invention:

- Components used in the fluid path, and air contained within each is sterilised during manufacture.
- There is usually a small void of air or gas in bottles of medical fluid.
- Before tapping, the protective cap over the bung centre is removed (to allow access
25 to for the spike), however the bung retainer 1025 (shown in Figure 24) is left on the bottle (otherwise the bung may be dislodged by air pressure during filling).
- Injector syringes are typically supplied fitted with the plunger retracted (i.e. it is filled with sterile air)

- The syringe, tube, and spike would have standard luer locking connectors to ensure they are secure and sealed under pressure.

The following variations to the system could enhance the invention under some circumstances:

- 5 • The Fill sequence program could be extended with an additional forward-retract cycle – particularly for volumes approaching the maximum capacity of the syringe. This is to ensure that all air has been expelled. When a syringe is to be filled to near capacity (>75%) there is insufficient travel on the piston to retract 130% . Hence additional strokes are required to expel all the air. This “130%” figure is a function
10 of the volume of (air) the tube, and air space in the bottle – a greater tube volume (or less air space in the bottle) requires more over travel.
- During the fill sequence, the first compression stroke of the piston would preferably expel all the air from the syringe – particularly for x-ray contrast, where the bottles normally have a significant air space.
- 15 • Alternatively, to optimise performance even with bottles having relatively small air space, during the compression the injector could sense the pressure in the system (for example by sensing the load on the drive means) and retract prematurely if the pressure approached unsafe levels.
- The controlling electronics and associated displays and audible enunciators could
20 prompt the operator as to what step or otherwise to take next in the filling routine.
- The injector tilt switches (or sensors) could be used to trigger or inhibit other functions of the injector, for example inhibit injection until the injector and syringe are oriented downward, or enable higher flow rates during fill (rates that would be unsafe for injecting into patients).
- 25 • The syringe 1014 could be supplied with the extension tube 1010 and spike 1014 already assembled (as shown in Figure 24) during manufacture, further reducing operator time.
- The Syringe 1014 and Tube 1010 could be manufactured with the tube 1010 permanently attached and bonded directly to the syringe tip 1012, protecting the

sterility of the syringe tip 1012, and reducing manufacturing & material costs by dispensing with connector 1013, which is normally used to adapt the tubing 1010 to the syringe tip 1012 (as illustrated in Fig's 31 to 33, and described below). As well, safety is improved by ensuring the tube cannot be disconnected, possibly releasing contaminated fluids.

- An air detector (optical, ultrasonic, etc) could be fitted to the tubing, ensuring there is no air present after filling, and disallowing operation of the injector until the air is removed.
- The syringe 1014 and associated extension tube 1010 could be permanently bonded 1039 to a special combination patient connector with frangible spike (as shown in Fig 27c.), and all supplied as one set 1060. This set could provide a reduced cost, as well as a non-reusable system which could prevent patient to patient cross-infection. This concept is described in detail as follows:

The complete set 1060 (as shown in Figure 28) is used to fill the syringe much as described previously, however after filling is complete, instead of disconnecting the spike from the tube, spike 60 is then snapped off, and as before, leaves a male luer connector on the end of the tube for connection to the patient. Importantly however, with the spike removed the syringe is less likely to be inadvertently re-filled, and hence cannot be used with more than one patient, thus preventing cross-infection from one patient to the next.

It is understood that a conventional spike can still be attached after the frangible spike is removed and therefore used to re-fill, and possibly cause contamination. This could be overcome by adopting a non-standard connector (eg larger diameter Luer). This would require a non-standard mating connector on the needle. Also, if the contents of a bottle are used to fill more than one syringe (as is often the case) the bottle cannot be inadvertently contaminated by re-filling a used syringe.

Figures 26 and 27 show various examples 1040 and 1050 of combination male luer connector with frangible spikes and tube 1010. Figure 28 shows the complete set 1060 having an extension tube 1010 bonded at each end to the syringe 1014 and frangible connector/spike 1050.

The alternative combination connector/spikes are illustrated and described as follows:

Figures 26a to 26d show various views of an example of a combination 1040 of male Luer connector 1046 with frangible spike 1042, and locking collar 1047. Figure 26a is an oblique view of combination Luer connector 1046 with frangible spike 1042 and locking collar 1047 before assembly. Disc 1043 simply provides a grip for holding the spike. The frangible neck 1044 is seen clearly in Figure 26b, which is a longitudinal axial cross-section view of a combination Luer connector 46 with frangible spike 1042 and locking collar 1047, after assembly. The locking collar has a conventional female luer locking thread for retaining the patient needle, which is connected after the spike is detached. Small raised nodules or barbs 1048 serve as detents to discourage the collar from sliding off the connector once assembled. The locking collar 1047 is not essential to the invention, however is advisable when used with pressure injectors.

Figure 26c shows a side view of the combination connector/spike/collar 1040, after assembly and bonding to the tube 1010.

Figure 26d shows a combination connector/spike/collar 1040 after the spike has been detached at the frangible neck 1044, leaving a standard male luer lock connector 1046 on the end of the tube 1010.

Figures 27a to 27c show various views of an alternate example of a combination 1050 of male Luer connector 1046 with barbed frangible spike 1051, and locking collar 1047. The barbs 1053 are useful in discouraging the spike from being dislodged from the bung 1025 of the bottle 1026 during the pressurization phase of filling.

Figure 27a shows a longitudinal axial cross-section view of combination 1050 connector/barbed frangible spike/collar.

Figure 27b shows combination 1050 connector/barbed frangible spike/collar, after assembly and bonding to the tube 1010.

Figure 27c shows a shorter example of combination 1050 connector/barbed frangible spike/collar. It will be appreciated by those familiar with the art that the spike may well be significantly shorter (in proportion) depending on the size of the bottle and bung.

Figure 28 shows an example of combination 1060 connector/barbed frangible spike/collar permanently bonded to the associated Extension Tube 1010 and Syringe 1014, to form a non re-usable set 1060 for injecting patients.

The complete set 1060 is used as follows: Firstly the spike 1051 is inserted into the bung (not shown in Figure 28), and the syringe 1014 is filled as previously described. After the spike 1051 is withdrawn from the bung, the spike end 1051 is “snapped off” at the frangible neck 1044 and discarded, leaving the conventional male luer lock tip 1046 for connection to the patient (not shown). It should be noted that the patient (not shown) cannot possibly be connected to the set 1041 until the spike 1051 is detached. Once separated however, the spike 1051 cannot ordinarily be reconnected, and hence associated tube 1010 and syringe 1014 cannot be re-filled, thus ensuring only one patient can be injected per set – ie this prevents any chance of inadvertent cross infection from one patient to the next.

It would be appreciated by those familiar with the art that a vented spike could also be combined frangibly with a male luer connector, however the syringe would be filled in a more conventional manner.

It should be noted that all cross-section views in Figures 29 to 33 are longitudinal, through the axis of the parts.

As required above and elsewhere in medicine, it is often desirable to connect or bond a flexible plastic tube directly to a rigid plastic spout or luer outlet. A typical male Luer Lock connection is illustrated in Figure 29, before connection. Figure 29a shows an overall view, and Figure 29b shows a longitudinal axial cross-section view. The syringe body 2010 has an outlet connector tip 2011 which has a tapered male luer outer surface 2014, surrounded by a female locking thread 2012 of larger diameter, on the same axis but slightly forward of the thread. It should be noted that almost all luer tapers 2014 are made to a standard diameter, with a taper of approximately 6% as defined in International Standard ISO594. The outer luer taper 2014 is clearly evident in cross-section Figure 29b. Syringes 2010 (including tip 2011 and thread 2012) are normally injection moulded from tough semi-rigid transparent polypropylene.

Figure 30 illustrates a soft plastic tube 2016 pushed fully over the syringe tip 2011. The tip 2011 has a tapered outer 2014, and the tubing 2016 stretches and conforms to the taper 2014, and the resultant outer surface 2018 of the tubing forms an enlarged taper.

In Figure 31 the basic form of clamp invention is shown before and after fitting.

The clamp 2020 is formed in a cylindrical shape with a hollow inner tapered diameter 2021 from semi rigid plastic, with a small chamfer 2022 on the leading edge to assist assembly. The clamp 2020 is installed by simply pushing over the tapered outer surface 2018 of the tube, and inside the female thread 2012 of the syringe connection. It will be understood by those familiar with the art that the clamp 2020 has suitably precise dimensions for a firm interference fit on both its inner and outer diameters, as illustrated, to suit the wall thickness and compliance of both the tubing and the syringe.

When force fitted, the inner taper 2021 of clamp 2020 firmly squeezes the tubing 2016 onto the tip 2011 of the syringe 2010, as shown in Figure 31. The syringe tip 2011 is also made from semi-rigid plastic, and all components deform slightly to exert even pressure on the luer tip/tube connection, ensuring it is sealed very effectively.

Alternate variations to the basic clamp design are illustrated in Figures 32 to 35.

In Figure 32 small barbed annular rings 2032 have been added to the outer surface of the barbed clamp 2030 to improve retention inside the female locking thread of the connector. The clamp 2030 is pressed over the tube 2016 and into the syringe 2010 as above, and the barbs 2032 interfere with and grip the female thread 2012 ensuring it cannot be dislodged. As above, inner taper 2021 of clamp 2030 firmly squeezes the tubing 2016 onto the tip 2011 of the syringe 2010. This type of clamp would suit permanent and tamperproof applications because the clamp would be almost impossible to remove without the use of tools.

In Figure 33, male threads 2042 have been added to the outer surface of two similar styles of clamp 2040 and 2050, which mate with the female thread 2012 of the syringe 2010, and have a tapered inner surface 2021. The purpose of thread 2042 is to assist assembly, as well as firmly clamp the tube 2016 onto luer taper 2014. During assembly the clamps 2040 or 2050 are simultaneously pushed and screwed inside the syringe thread 2012 and over the tube 2016, squeezing the tube 2016 onto the luer taper 2014, resulting in a more secure, tighter fitting connection than those described above. As above, inner taper 2021 of clamps 2040 and 2050 firmly squeezes the tubing 2016 onto the tip 2011 of the syringe 2010.

Figure 33b has additional barbed serrations 2054 to the rear end of the clamp, which assist in gripping and twisting the clamp during assembly.

It will be understood by those familiar with the art that the rear end or flange may take many forms to suit hand, machine, or tooled assembly, and /or to discourage disassembly.

Figure 33c shows a longitudinal cross-section of either clamp 2040 or 2050, showing male threads 2042, and internal taper 2021 to mate with outer taper 2018 of tube 2016.

5 Figure 33d shows a longitudinal cross-section of either clamp 2040 or 2050,

Figure 33e shows a longitudinal cross-section of clamp 2060, showing male threads 2042, plus an internal annular ridge 2062 added to the inside surface of the ridged clamp 2060.

Figure 33f shows clamp 2060 after being simultaneously pushed and screwed inside the syringe thread 2012 and over the tube 2016, squeezing the tube 2016 onto the luer taper 2014. The internal ridge 2062 of clamp 2060 concentrates the squeezing action to a short area 2064 [not seen in Figure 33f] of the union with the tube 2016, providing a more concentrated pressure and improved sealing compared with those described above. Alternately, it could be argued by those familiar with the art that clamp 2060 provides an equivalent seal to those above, with less assembly (and disassembly) force.

10

15 It will be understood by those familiar with the art that one or more annular rings may be included on the inner surface of any of the above clamp styles, and that the profile of the ridge may be varied to suit the hardness of the particular tubing employed (not illustrated).

Figures 34 and 35 illustrate various flanges 2072 and 2082 (respectively) added to the rear end of the threaded clamp style 2040 previously shown in Figure 33a. Both clamps 2070 and 2080 have male threads 2042 on their outer surface to mate with syringe female thread 2012, for the purpose of assisting assembly and firmly clamping the tube 2016. Figure 35 has additional barbed teeth 2082 on the outer perimeter of the flange 2083 which assist clockwise tightening 2084 of the clamp 2080, but hinder anti-clockwise unscrewing, thereby making the connection virtually tamperproof. Both clamps 2070 and 2080 are inserted into the syringe (and clamp the tube) in the same manner as those described above, and may or may not have annular rings on their inner surface.

20

25

If a removable clamp is required, clamp 2070 in Figure 34 would be preferred. Alternatively the flange of clamp 2070 could have non-directional serrations added to assist grip in either direction (not illustrated).

Alternatively, a clamp of style 2080 in Figure 35b, but having barbs oriented opposite to those on clamp 2080 would ensure the clamp is not over-tightened, as well as improve the likelihood that the clamp could always be removed (not illustrated).

Figure 36 illustrates a side perspective view of a syringe holder with an engagement
5 portion to enable releasable engagement with a medical injector and sensing system to detect the presence of the syringe. Syringe holder 200 is engaged in injector nose 10 of the medical injector (not shown). Bayonet posts 3010 and a blocking member (holder lock post 3015) on injector nose 10 form part of the engagement mechanism between syringe
10 holder 200 and the injector. Syringe 300 is loaded into holder 200 and retained by catch 500. The injector nose 10 has a sensor or switch 3110 for sensing the presence of a syringe in holder 200. According to the embodiment illustrated, it is an optical sensor.

Holder lock post 3015 is adjacent to syringe sensor 3110 and therefore syringe holder 200 cannot be removed whilst a syringe is installed, nor during an injection. Additionally, a syringe cannot be installed unless holder 200 is locked fully (in this case clockwise). This
15 embodiment is particularly useful in the absence of a sensor to verify syringe presence. It will be appreciated that holder 200 could not be attached if a syringe were already installed.

To engage syringe holder 200 with injector nose 10, the holder is first inserted into the nose and with gentle inwards pressure, rotated until grooves 3020 (as shown in figure 37a)
20 engage bayonet posts 3010. At this point holder 200 fully enters the nose 10, and the holder is rotated to lock it in place. Whilst 3 bayonet groove/post sets are illustrated spaced evenly around the circumference, they could also be oriented at matching odd angles so that the holder can only engage in a particular orientation. Seal 3145 could be a simple O-ring or wiper ring, and has 2 important roles:

- 25 (a) prevent fluids from entering the injector
- (b) provide a friction means to decrease the possibility of inadvertent removal of the holder.

Figures 37a-d and 38 a-e illustrate several views of a syringe holder with a bayonet attachment 3010, a blocking member (holder lock post 3015), loaded syringe and sensing
30 system to detect the presence of a syringe. Injector nose 10 is fitted with a fluid seal 3145,

a spring stop ring 3140 against which syringe flag spring 3130 abuts. A syringe stop and plunger bush 3135 sits within injector nose 10 and syringe 300 briefly engages bush 3135 to limit movement of the syringe 300 towards the medical injector. Bush 3135 has at least one groove 3150 in which tabs 3122 (as depicted in figure 37c), are slidingly engaged.

5 Spring 3130 is compressed during assembly between stop ring 3140 and Tabs 3122 on Flag 3120, thereby biasing Flag 3120 forward (to the right). With no syringe installed Tabs 3122 rest against Bush 3135, and the pointed tip of Flag 3120 protrudes to the right of bush 3135.

Syringe holder 200 with grooves 3020 are introduced into injector nose 10 and the groove

10 is engaged with pins 3010 and rotated to thereby lock it in place. When syringe barrel 300 is inserted into holder 200, it depresses syringe flag 3120 and thus pushes tabs 3122 of the flag against spring 3130. Biased catch 500 snaps shut and locks syringe 300 in place within the holder.

Holder lock post 3015 is of similar width to, and mounted on the same axis, as flag 3120.

15 As holder 200 is attached, flag 200 almost touches it (the lock post?) when bayonet slots 3020 are fully engaged with posts 3010 (without rotating). In the mounted position, with a syringe installed and flag 3020 pushed back, holder 200 cannot be rotated the wrong way (in the present case anti-clockwise) because the flag 200 will engage the lock post 3015 and thereby prevent rotation of the holder 200 within the injector nose 10.

20 Flag 3120 has a beveled tip 3124 to engage syringe 300 and thereby grip it to minimize rotational movement. The movement of flag 3120 towards the injector triggers sensor 3110 which thereby creates a signal to the effect that a syringe is present in the holder. In the present case, sensor 3110 is a combination light emitter and detector sensing light reflected off the metallic surface of Flag 3120. The signal created may go to a controller

25 which thereby integrates the information and controls the movement of the syringe plunger 130. For example, the controller may restrict movement of the plunger until after the sensor creates a signal that a syringe is present. When syringe 300 is removed from holder 200, spring 3130 pushes flag 3120 away from sensor 3110 and thereby eliminates the reflections.

30 During assembly of holder 200 onto injector nose 10, bush 3135 and spring stop 3140 are normally fixed in place inside the holder by means of cement, screws, or pins. Both stops

have a small longitudinal groove 3150 in their outer surfaces to support slidable syringe flag 3120 which, together with flag spring 3130, are held in place by bush 3135 and stop 3140. Spring 3130 is lodged between spring stop 3140 and tabs 3122, thereby biasing the flag forward. With no syringe loaded, flag 3120 protrudes forward of the syringe stop 3135, and its tabs lodge against the rear of the syringe stop. A secondary function of the syringe stop is to bear and centre the plunger, and prevent stray fluid around the syringe from entering the injector.

In brief, the Syringe Flag device has 3 main functions:

1. Syringe ejector: Flag 3120 is slidably mounted in groove 3150, and is biased forward by flag spring 3130. As syringe 300 is loaded into holder 200 the rear rim strikes the flag, pushing it rearward and compressing the spring until the tip of the flag is flush with bush 3135. When catch 500 is opened, syringe 300 is partially ejected forward by the flag, making the syringe easier to grasp and remove.
2. When a tube is attached to the syringe (after it has been loaded), the operator needs to twist the connection to engage and lock the connection to the syringe thread. To restrain the syringe from rotating it would ordinarily need to be held with the other hand. However flag 3120 can perform this role. The forward tip 3124 of flag 3120 is beveled & sharp like a chisel, digging into the syringe a little, thereby restraining rotation of the syringe.
3. The flag assists detection of the presence of a syringe in holder 200. Reflective infrared sensors such as Sharp GP2L24 are readily available types of sensors 3110. As the flag is pushed back by the syringe the reflective rear end of the flag is detected by the sensor, which in turn signals the controller. Those familiar with the art will appreciate that various other forms of detection or mechanical switching could be used to sense movement of the Flag 3120.

Figures 39a & b illustrate cross sectional views of a syringe in a syringe holder demonstrating a particularly preferred embodiment of the engagement mechanism between the hub and plunger.

Plunger 3600 is slidably engaged with actuation member 3610 but with a limited free play between them due to space 3625. Note also that free sliding of plunger 3600 is somewhat

subdued by the seal 3146. Whenever drive member 3500 and actuation member 3610 reverse direction, plunger 3600 does not move until space 3625 is traversed. Actuation member 3610 and its associated cone 3650 operate pins 3640 to automatically engage or disengage hub 310 at the appropriate time.

- 5 Holder 200 is engaged in injector nose 10. Syringe 300 has been fitted into holder 200. Figure 39a demonstrates this embodiment in the situation where the plunger is expelling fluid from the syringe. Shoulder 3520 of plunger drive 3500 engages and pushes plunger 3600 and actuation member 3610 which is disposed within a bore in plunger 3600. Actuation member 3610 has a rod portion 3165 [not seen ;labeled in Fig. 39] and a nose
- 10 portion 3650 which is cone shaped. The forward movement of nose portion 3650 allows locking members in the form of pins 3640 which are biased by spring 3660 to retract from engagement with the engagement portion of hub 310. Thus hub 310 is automatically unlocked during and following forward movement of plunger 130. The purpose of unlocking the hub is to allow removal of the used syringe following an injection.
- 15 On retraction of plunger drive 3500, shoulder 3520 of plunger drive 3500 withdraws from the rear edge of plunger 3600 and thereby actuation member 3610 is drawn away from hub 310. Plunger 3600 is momentarily stationary, causing nose portion 3650 to slide along pins 3640 and thereby force them to extend from plunger 3600 and engage the engaging portion of the hub 310. Shoulder 3630 on actuation member 3610 traverses space 3625 and
- 20 engages shoulder 3620 in the bore and enables nose portion 3650 to be positioned alongside pins 3640 by stopping actuation member 3610 from moving relatively further away from them. Thus hub 310 is automatically retained during and following retraction movement of plunger drive 3500 , enabling retraction of the hub, and filling of the syringe.

Hence this system automatically ensures that the hub is either locked or unlocked at the

- 25 appropriate time, avoiding inconvenience and enhancing safety of the injector - for the operator and the patient. Of course, the Controller must be programmed to allow for the inherent free play whenever the plunger reverses direction.

Figure 40 illustrates a longitudinal cross sectional view of a plunger and hub demonstrating a preferred embodiment of the sensor to detect engagement between the hub and plunger.

- 30 Syringe 300 has a hub 310 slidably disposed within it. Sensor 3300 is a light sensor with an optical fibre cable 3350 which is partially embedded in plunger 130. Optical fibre 3350

has an exposed end 3355 which is flush with the surface of plunger 130 and detects incident light 3360 which passes through transparent syringe 300. Incident light is then transmitted 3365 along optical cable 3350. When plunger 130 has fully engaged hub 310, which is opaque, incident light will not be able to hit the end of optical cable 3350.

5 Therefore, the light sensor 3360 will detect the absence of light and create an appropriate signal. Of course, if the room lights are inadequate for the sensor to operate, the Plunger can be illuminated by the injector with visible or infrared light.

This signal may be sent to a controller via cable 3370 to enable further control over the movement of plunger 130. For example, it may allow plunger 130 to automatically stop

10 upon full engagement with hub 310 without thereby causing hub 310 to be moved forward. According to this embodiment, since the aperture at the end of the optic fibre is small, then the ambient light is cut off abruptly as the plunger enters the hub, and so the accuracy and predictability of the system is enhanced. Similarly, because of the high contrast between the engaged and non-engaged states, the level of ambient or illuminated light is not critical.

15 Figures 41 & 42 illustrate one embodiment of the medical injector with tilt switches in the injecting and filing positions. Injector Head 4000 contains the control and drive elements of the Injector and is mounted at Head Pivot 4050 to Injector Pedestal 4100, which preferably stands on a wheeled base (not shown). Head 4000 is able to tilt about the pivot by at least 90 degrees.

20 A small Switch Tab 4030 extends from Injector Pedestal 4030. Switches 4010 and 4020 are fixed to the head in such positions as to strike the Switch Tab at the opposing positions of DOWN (4020) and UP (4010), at which points the appropriate switch changes state, and communicates to the Control circuitry (not shown) the orientation of head 4000. These communications can be used to initiate or inhibit a plurality of functions, operations,

25 displays, responses, and/or safeguards in the injector.

Those familiar with the art will appreciate that various alternate sensors could be used in place of Switches 4010 and 4020, such as magnetic, optical, or mechanical. It will also be noted that a plurality of Tabs and Switches may be used to sense multiple orientations of the head.

30 It should also be noted that the above concepts operate without regard to earth's gravitation.

It will be understood by those familiar with the art that the inventions described above could be applied to any standard male luer locking connector, as found on many medical and other devices. It will also be understood that various combinations of outer and inner surfaces, combined with any of the above mentioned rear ends or flanges are possible, depending on the application.

The word 'comprising' and forms of the word 'comprising' as used in this description do not limit the invention claimed to exclude any variants or additions.

Modifications and improvements to the invention will be readily apparent to those skilled in the art. Such modifications and improvements are intended to be within the scope of this invention.

THE CLAIMS DEFINING THE INVENTION ARE AS FOLLOWS:

- 1 A syringe holder for a medical injector system comprising:
 - (i) a cradle member adapted to receive a barrel of the syringe; and
 - (ii) a pivotable catch to releasably lock the syringe in the cradle member
- 5 wherein the catch is biased towards a first position and engages the syringe at the first position and disengages the syringe at a second position.
- 2 A syringe holder according to claim 1 comprising a positioning device located on the cradle member to locate one end of the syringe in a predetermined location in the cradle member.
- 10 3 A syringe holder according to claim 1 wherein the cradle member is a sleeve.
- 4 A syringe holder according to claim 3 wherein the sleeve is adapted to support the syringe against expansion under pressure.
- 5 A syringe holder according to claim 1 wherein the catch engages a front shoulder of the syringe.
- 15 6 A syringe holder according to claim 1 wherein the catch engages the syringe through a hole defined in the cradle member.
- 7 A syringe holder according to claim 1 wherein the cradle member has a biasing member to partially eject the syringe from the cradle member upon release of the catch.
- 20 8 A syringe holder according to claim 7 wherein the biasing member comprises a spring.
- 9 A syringe holder according to claim 7 wherein the biasing member is adapted to engage and minimise rotation of the syringe.
- 10 A syringe holder according to claim 1 wherein the front shoulder of the syringe is
- 25 of a complimentary shape to an engaging portion of the catch.
- 11 A syringe holder according to claim 10 wherein the engaging portion of the catch is concave.

- 12 A syringe holder according to claim 10 wherein the engaging portion of the catch is convex.
- 13 A syringe holder according to claim 10 wherein the catch is wedge shaped.
- 14 A syringe holder according to claim 1 wherein it comprises an engagement portion
5 to enable simple releasable engagement with a medical injector.
- 15 A syringe holder according to claim 14 wherein the engagement portion comprises a locking member.
- 16 A syringe holder according to claim 15 wherein the locking member comprises a slot.
- 10 17 A syringe holder according to claim 15 wherein the locking member comprises a pin.
- 18 A syringe holder according to claim 15 comprising a blocking member to regulate disengagement of the holder from the medical injector.
- 19 A syringe holder according to claim 18 wherein the blocking member stops
15 disengagement of the holder from the medical injector if a syringe is present in the holder.
- 20 A syringe holder according to claim 18 wherein the blocking member stops disengagement of the holder from the medical injector if the plunger is not in a particular position.
- 20 21 A syringe holder according to claim 19 wherein the blocking member stops disengagement of the holder from the medical injector if the plunger is not in a sufficiently retracted state.
- 22 A syringe holder according to claim 1 for use with a medical injector system according to claim 183.
- 25 23 A syringe holder according to claim 1 for use with a medical injector system according to claim 189.
- 24 A syringe holder according to claim 1 for use with a medical injector system according to claim 193.

- 25 A syringe holder according to claim 1 for use with a medical injector system according to claim 201.
- 26 A syringe holder according to claim 1 for use with a medical injector system according to claim 205.
- 5 27 A syringe holder according to claim 1 for use with a medical injector system according to claim 213.
- 28 A syringe holder according to claim 1 for use with a syringe according to claim 154.
- 29 A syringe holder according to claim 1 for use with a syringe according to claim 155.
- 10 30 A method of filling a syringe with medical fluid from a sealed vessel the syringe for use with a medical injector system comprising a syringe holder according to claim 1, comprising the steps of:
- 15 (i) elevating the front portion of the syringe relative to the back portion;
- (ii) advancing a plunger to a position within the syringe corresponding to a predetermined patient dose;
- (iii) controlling movement of the plunger in a sequence of forward and backward movements to expel air from the syringe and any attached tube into the vessel bottle, and draw the desired dose of fluid into the syringe.
- 20 31 A method of filling a syringe according to claim 30 further comprising the step of automatically restricting the direction of movement of the plunger depending on the orientation of the syringe.
- 32 A method of filling a syringe according to claim 31 wherein the plunger may move either forward or backward when oriented with its front portion elevated with respect to its back portion and only in the forward direction when oriented with the back portion elevated with respect to its front portion.
- 25 33 A method of injecting a patient using a medical injector system comprising a syringe holder according to claim 1 comprising the steps of;
- (i) engaging a plunger with a hub slidably engaging the barrel of a syringe

- (ii) driving the hub along the syringe barrel; and
 - (iii) expelling fluid from the syringe into a patient.
- 34 A method for engaging a syringe holder according to claim 14 with a medical injector, comprising the steps of;
 - 5 (i) aligning the engaging portion of the syringe holder with a complimentary portion on the medical injector; and
 - (ii) engaging the syringe holder with the medical injector.
- 35 A method for disengaging a syringe holder according to claim 14 from a medical injector, comprising the steps of;
 - 10 (i) disengaging the engaging portion of the syringe holder from the medical injector; and
 - (ii) removing the syringe holder from the medical injector.
- 36 A method for loading a syringe into a syringe holder according to claim 1, comprising the steps of;
 - 15 (i) inserting a syringe barrel in the cradle member such that the catch is displaced; and
 - (ii) allowing the catch mechanism to return into its biased position to engage the syringe and thereby retain the syringe in the cradle member.
- 37 A method for removing a syringe, from a syringe holder according to claim 1
20 comprising the steps of;
 - (i) releasing the catch to unlock the syringe; and
 - (ii) withdrawing the syringe from the cradle member.
- 38 A syringe holder according to claim 1 for use with a syringe comprising a hub according to claim 43.
- 25 39 A syringe holder according to claim 1 for use with a plunger according to claim 74.

- 40 A syringe holder according to claim 1 for use with a plunger according to claim 109.
- 41 A syringe holder according to claim 1 for use with a sensing system according to claim 157.
- 5 42 A syringe holder according to claim 1 for use with a sensing system according to claim 166.
- 43 A hub for a syringe for use with a medical injector system, comprising an outer surface adapted to slidably engage with a barrel of the syringe, and an inner surface having a substantially annular engaging portion adapted to be releasably engaged by a plunger to permit the hub to be selectively withdrawn along the barrel by the plunger.
- 10 44 A hub according to claim 43 wherein the engaging portion defines a cavity.
- 45 A hub according to claim 43 wherein the engaging portion comprises a groove.
- 46 A hub according to claim 45 wherein the groove extends at least partially along the circumference of the inner surface of the hub.
- 15 47 A hub according to claim 43 wherein the engaging portion is a ridge.
- 48 A hub according to claim 43 wherein the inner surface of the hub is complementary in shape to an outer surface of the plunger.
- 49 A hub according to claim 48 wherein the inner surface comprises an interior hollow that contacts the plunger.
- 20 50 A hub according to claim 43 wherein the hub comprises a seal.
- 51 A hub according to claim 50 wherein the seal has an extended leading edge to increase the efficiency of the seal under pressure.
- 52 A hub according to claim 43 for use with a medical injector system according to claim 183.
- 25 53 A hub according to claim 43 for use with a medical injector system according to claim 189.

- 54 A hub according to claim 43 for use with a medical injector system according to claim 193.
- 55 A hub according to claim 43 for use with a medical injector system according to claim 201.
- 5 56 A hub according to claim 43 for use with a medical injector system according to claim 205.
- 57 A hub according to claim 43 for use with a medical injector system according to claim 213.
- 58 A hub according to claim 43 for use with a syringe according to claim 154.
- 10 59 A hub according to claim 43 for use with a syringe according to claim 155.
- 60 A method of filling a syringe with medical fluid from a sealed vessel the syringe comprising a hub according to claim 43, comprising the steps of:
- 15 (i) elevating the front portion of the syringe relative to the back portion;
- (ii) advancing a plunger to a position within the syringe corresponding to a predetermined patient dose;
- (iii) controlling movement of the plunger in a sequence of forward and backward movements to expel air from the syringe and any attached tube into the vessel bottle, and draw the desired dose of fluid into the syringe.
- 61 A method of filling a syringe according to claim 60 further comprising the step of
- 20 automatically restricting the direction of movement of the plunger depending on the orientation of the syringe.
- 62 A method of filling a syringe according to claim 61 wherein the plunger may move either forward or backward when oriented with its front portion elevated with respect to its back portion and only in the forward direction when oriented with the
- 25 back portion elevated with respect to its front portion.
- 63 A method of injecting a patient using syringe comprising a hub according to claim 43 and a medical injector system comprising the steps of;
- (i) engaging a plunger with a hub slidably engaging the barrel of a syringe

- (ii) driving the hub along the syringe barrel; and
 - (iii) expelling fluid from the syringe into a patient.
- 64 A method for loading a syringe comprising a hub according to 43 into a syringe holder, comprising the steps of;
 - 5 (i) inserting a syringe barrel in the cradle member such that the catch is displaced; and
 - (ii) allowing the catch mechanism to return into its biased position to engage the syringe and thereby retain the syringe in the cradle member.
- 65 A method for removing a syringe comprising a hub according to 43, from a syringe holder comprising the steps of;
 - 10 (i) releasing the catch to unlock the syringe; and
 - (ii) withdrawing the syringe from the cradle member.
- 66 A method of connecting a syringe hub according to claim 43 to a plunger according to claim 74 comprising the steps of;
 - 15 (i) introducing the plunger into a syringe barrel within which the hub is slidingly engaged and engaging the plunger with the inner surface of the hub; and
 - (ii) activating the plunger such that the retention member engages the engaging portion of the hub.
- 20 67 A method for hand filling a syringe comprising a hub according to claim 43 and a plunger according to claim 74 comprising the steps of;
 - (i) introducing the plunger into the syringe barrel and engaging the plunger with the inner surface of the hub;
 - (ii) activating the plunger such that the retention member engages the engaging portion of the hub; and
 - 25 (iii) withdrawing the engaged hub along the syringe barrel whilst drawing liquid into the syringe.

- 68 A hub according to claim 43 for use with a syringe holder according to claim 1.
- 69 A hub according to claim 43 for use with a plunger according to claim 74.
- 70 A hub according to claim 43 for use with a plunger according to claim 109.
- 71 A hub according to claim 43 for use with a device according to claim 136.
- 5 72 A hub according to claim 43 for use with a sensing system according to claim 157.
- 73 A hub according to claim 43 for use with a sensing system according to claim 166.
- 74 A plunger for a syringe for use with a medical injector system, the syringe having a
barrel and a hub slidingly engaging the barrel, the plunger comprising a retention
member adapted to releasably engage a substantially annular engaging portion on
10 an inner surface of the hub to permit the hub to be selectively withdrawn along the
barrel by the plunger.
- 75 A plunger according to claim 74 wherein the retention member is mechanically
and/or electrically releasably engaged with the hub.
- 76 A plunger according to claim 75 wherein the releasable engagement is at least
15 partly actuated by a weight mechanism.
- 77 A plunger according to claim 74 wherein the releasable engagement is actuated by
retraction of the plunger.
- 78 A plunger according to claim 74 wherein the retention member is biased away from
engagement with the hub.
- 20 79 A plunger according to claim 74, wherein the retention member comprises an
actuation member disposed at least partially within a bore defined in the plunger
and a locking member is located at or adjacent one end of the retention member
and/or plunger, the locking member being movable by the retention member into or
out of engagement with the engaging portion of the hub.
- 25 80 A plunger according to claim 79 wherein the retention member comprises a cam.
- 81 A plunger according to claim 79 wherein the retention member comprises a cone.

- 82 A plunger according to claim 79, wherein the actuation member has a rod portion and a nose portion and the locking member is, in the unlocked position, located between the plunger and the nose portion.
- 5 83 A plunger according to claim 79 wherein the actuation member is movable longitudinally along the bore in the plunger.
- 84 A plunger according to claim 74 wherein the retention member comprises a pin.
- 85 A plunger according to claim 74 adapted for manual filling of the syringe.
- 86 A plunger according to claim 85 wherein the plunger is incapable of engaging the hub after the syringe has been used.
- 10 87 A plunger according to claim 86 wherein the plunger is sufficiently shorter than the barrel of the syringe such that it can not reach the hub when the hub is located at the front most portion of the syringe barrel.
- 88 A plunger according to claim 74 for use with a medical injector system according to claim 183.
- 15 89 A plunger according to claim 74 for use with a medical injector system according to claim 189.
- 90 A plunger according to claim 74 for use with a medical injector system according to claim 193.
- 91 A plunger according to claim 74 for use with a medical injector system according to claim 201.
- 20 92 A plunger according to claim 74 for use with a medical injector system according to claim 205.
- 93 A plunger according to claim 74 for use with a medical injector system according to claim 213.
- 25 94 A plunger according to claim 74 for use with a syringe according to claim 154.
- 95 A plunger according to claim 74 for use with a syringe according to claim 155.

- 96 A method of filling a syringe with medical fluid from a sealed vessel using a medical injector system, the system comprising a plunger according to claim 74, comprising the steps of:
- 5 (i) elevating the front portion of the syringe relative to the back portion;
- (ii) advancing a plunger to a position within the syringe corresponding to a predetermined patient dose;
- (iii) controlling movement of the plunger in a sequence of forward and backward movements to expel air from the syringe and any attached tube into the vessel bottle, and draw the desired dose of fluid into the syringe.
- 10 97 A method of filling a syringe according to claim 96 further comprising the step of automatically restricting the direction of movement of the plunger depending on the orientation of the syringe.
- 98 A method of filling a syringe according to claim 97 wherein the plunger may move either forward or backward when oriented with its front portion elevated with
- 15 respect to its back portion and only in the forward direction when oriented with the back portion elevated with respect to its front portion.
- 99 A method of injecting a patient using medical injector system comprising a plunger according to claim 74 comprising the steps of;
- (i) engaging a plunger with a hub slidably engaging the barrel of a syringe
- 20 (ii) driving the hub along the syringe barrel; and
- (iii) expelling fluid from the syringe into a patient.
- 100 A method for loading a syringe into a syringe holder in a medical injector system comprising a plunger according to 74, comprising the steps of;
- (i) inserting the syringe barrel in the cradle member such that the catch is
- 25 displaced; and
- (ii) allowing the catch mechanism to return into its biased position to engage the syringe and thereby retain the syringe in the cradle member.
- 101 A method for removing a syringe from a syringe holder in a medical injector system comprising a plunger according to 74, comprising the steps of;

- (i) releasing the catch to unlock the syringe; and
 - (ii) withdrawing the syringe from the cradle member.
- 102 A method of connecting a syringe hub according to claim 43 to a plunger according to claim 74 comprising the steps of;
- 5 (i) introducing the plunger into a syringe barrel within which the hub is slidingly engaged and engaging the plunger with the inner surface of the hub; and
- (ii) activating the plunger such that the retention member engages the engaging portion of the hub.
- 10 103 A method for hand filling a syringe comprising a hub according to claim 43 and a plunger according to claim 74 comprising the steps of;
- (i) introducing the plunger into the syringe barrel and engaging the plunger with the inner surface of the hub;
- (ii) activating the plunger such that the retention member engages the engaging portion of the hub; and
- 15 (iii) withdrawing the engaged hub along the syringe barrel whilst drawing liquid into the syringe.
- 104 A plunger according to claim 74 for use with a syringe holder according to claim 1.
- 105 A plunger according to claim 74 for use with a syringe comprising a hub according to 43.
- 20 106 A plunger according to claim 74 for use with a device according to claim 136.
- 107 A plunger according to claim 74 for use with a sensing system according to claim 157.
- 108 A plunger according to claim 74 for use with a sensing system according to claim 166.
- 25 109 A plunger for a syringe for use with a medical injector system, the syringe having a barrel and a hub slidingly engaging the barrel, the plunger comprising:

- (i) a retention member adapted to releasably engage an engaging portion of the hub to permit the hub to be selectively withdrawn along the barrel by the plunger; and
 - (ii) a sensor to detect a level of engagement between the plunger and the hub.
- 5 110 A plunger according to claim 109 wherein the sensor detects full engagement between the plunger and hub.
- 111 A plunger according to claim 109 comprising a light sensor.
- 112 A plunger according to claim 111 wherein the light sensor comprises a fibre optic cable.
- 10 113 A plunger according to claim 109 comprising a mechanical sensor.
- 114 A plunger according to claim 109 comprising an electromagnetic sensor.
- 115 A plunger according to claim 109 for use with a medical injector system according to claim 183.
- 15 116 A plunger according to claim 109 for use with a medical injector system according to claim 189.
- 117 A plunger according to claim 109 for use with a medical injector system according to claim 193.
- 118 A plunger according to claim 109 for use with a medical injector system according to claim 201.
- 20 119 A plunger according to claim 109 for use with a medical injector system according to claim 205.
- 120 A plunger according to claim 109 for use with a medical injector system according to claim 213.
- 121 A plunger according to claim 109 for use with a syringe according to claim 154.
- 25 122 A plunger according to claim 109 for use with a syringe according to claim 155.

- 123 A method of filling a syringe with medical fluid from a sealed vessel using a medical injector system, the system comprising a plunger according to claim 109, comprising the steps of:
- (i) elevating the front portion of the syringe relative to the back portion;
 - 5 (ii) advancing the plunger to a position within the syringe corresponding to a predetermined patient dose;
 - (iii) controlling movement of the plunger in a sequence of forward and backward movements to expel air from the syringe and any attached tube into the vessel bottle, and draw the desired dose of fluid into the syringe.
- 10 124 A method of filling a syringe according to claim 123 further comprising the step of automatically restricting the direction of movement of the plunger depending on the orientation of the syringe.
- 125 A method of filling a syringe according to claim 124 wherein the plunger may move either forward or backward when oriented with its front portion elevated with respect to its back portion and only in the forward direction when oriented with the back portion elevated with respect to its front portion.
- 15 126 A method of injecting a patient using medical injector system comprising a plunger according to claim 109 comprising the steps of;
- (i) engaging a plunger with a hub slidably engaging the barrel of a syringe
 - 20 (ii) driving the hub along the syringe barrel; and
 - (iii) expelling fluid from the syringe into a patient.
- 127 A method for loading a syringe into a syringe holder in a medical injector system comprising a plunger according to 109, comprising the steps of;
- (i) inserting the syringe barrel in the cradle member such that the catch is displaced; and
 - 25 (ii) allowing the catch mechanism to return into its biased position to engage the syringe and thereby retain the syringe in the cradle member.
- 128 A method for removing a syringe from a syringe holder in a medical injector system comprising a plunger according to 109, comprising the steps of;

- (i) releasing the catch to unlock the syringe; and
 - (ii) withdrawing the syringe from the cradle member.
- 129 A method of connecting a syringe hub according to claim 43 to a plunger according to claim 109 comprising the steps of;
- 5 (i) introducing the plunger into a syringe barrel within which the hub is slidingly engaged and engaging the plunger with the inner surface of the hub; and
- (ii) activating the plunger such that the retention member engages the engaging portion of the hub.
- 10 130 A method for connecting a syringe hub according to claim 129 further comprising the step of detecting a level of engagement between the plunger and the hub.
- 131 A plunger according to claim 109 for use with a syringe holder according to claim 1.
- 132 A plunger according to claim 109 for use with a syringe comprising a hub
15 according to 43.
- 133 A plunger according to claim 109 for use with a device according to claim 136.
- 134 A plunger according to claim 109 for use with a sensing system according to claim 154.
- 135 A plunger according to claim 109 for use with a sensing system according to claim
20 166.
- 136 A device for manually filling a syringe for use with a medical injector system, the syringe having a barrel and a hub slidingly engaging the barrel, the device comprising a plunger and a retention member adapted to releasably engage an engaging portion of the hub to permit the hub to be selectively withdrawn along the
25 barrel by the plunger.
- 137 A device according to claim 136 wherein the retention member is mechanically and/or electrically releasably engaged with the hub.

- 138 A device according to claim 136 wherein the releasable engagement is at least partly actuated by a weight mechanism.
- 139 A device according to claim 136 wherein the releasable engagement is actuated by retraction of the plunger
- 5 140 A device according to claim 136 wherein the retention member is biased away from engagement with the hub.
- 141 A device according to claim 136, wherein the retention member comprises an actuation member disposed at least partially within a bore defined in the plunger and a locking member is located at or adjacent one end of the retention member and/or plunger, the locking member being movable by the retention member into or
10 out of engagement with the engaging portion of the hub.
- 142 A device according to claim 141 wherein the retention member comprises a cam.
- 143 A device according to claim 141 wherein the retention member comprises a cone.
- 144 A device according to claim 141 wherein the actuation member has a rod portion
15 and a nose portion and the locking member is, in the unlocked position, located between the plunger and the nose portion.
- 145 A device according to claim 136 wherein the retention member comprises a pin.
- 146 A device according to claim 136 wherein the plunger is incapable of engaging the hub after the syringe has been used.
- 20 147 A device according to claim 136 wherein the plunger is sufficiently shorter than the barrel of the syringe such that it can not reach the hub when the hub is located at the front most portion of the syringe barrel.
- 148 A device according to claim 136 for use with a medical injector system according to claim 183.
- 25 149 A device according to claim 136 for use with a syringe according to claim 154.
- 150 A device according to claim 136 for use with a syringe according to claim 155.

- 151 A method of connecting a syringe hub according to claim 43 to a device according to claim 136 comprising the steps of;
- (i) introducing the device into a syringe barrel within which the hub is slidingly engaged and engaging the device with the inner surface of the hub; and
- 5 (ii) activating the device such that the retention member engages the engaging portion of the hub.
- 152 A method for hand filling a syringe comprising a hub according to claim 43 and a device according to claim 136 comprising the steps of;
- (i) introducing the device into the syringe barrel and engaging the device with the inner surface of the hub;
- 10 (ii) activating the device such that the retention member engages the engaging portion of the hub; and
- (iii) withdrawing the engaged hub along the syringe barrel whilst drawing liquid into the syringe.
- 15 153 A device according to claim 136 for use with a syringe comprising a hub according to 43.
- 154 A syringe for use with a medical injector system including the hub of claim 43.
- 155 A syringe for use with a medical injector system comprising a plunger according to claim 74.
- 20 156 A syringe for use with a medical injector system comprising a plunger according to claim 74 and a hub according to claim 43.
- 157 A sensing system for use with a medical injector system comprising a sensing member to detect the presence of a syringe holder associated with the medical injector system.
- 25 158 A sensing system according to claim 157 wherein the sensing member is a light sensor.

- 159 A sensing system according to claim 157 wherein the sensing member is a mechanical sensor.
- 160 A sensing system according to claim 157 wherein the sensing member is an electromagnetic sensor.
- 5 161 A sensing system according to claim 158 comprising a reflecting member to reflect light to the sensing member.
- 162 A sensing system according to claim 161 wherein the reflecting member is associated with the syringe.
- 10 163 A method for engaging a syringe holder according to claim 14 with a medical injector comprising the steps of;
- (i) aligning the engaging portion of the syringe holder with a complimentary portion on the medical injector; and
 - (ii) engaging the syringe holder with the medical injector.
 - (iii) detecting a level of engagement between the syringe holder and the medical injector system.
- 15
- 164 A method for disengaging a syringe holder according to claim 14 from a medical injector comprising the steps of;
- (i) disengaging the engaging portion of the syringe holder from the medical injector; and
 - (ii) removing the syringe holder from the medical injector
 - (iii) detecting a level of disengagement between the syringe holder and the medical injector system.
- 20
- 165 A method for modifying a medical injector system comprising the steps of:
- (i) replacing the syringe holder with a syringe holder according to claim 41
 - (ii) attaching a plunger according to claim 74.
- 25
- 166 A sensing system for use with a medical injector system comprising a sensing member to detect the presence of a syringe in a syringe holder associated with the

medical injector system wherein the sensing system is adapted for use with a removable syringe holder.

- 167 A sensing system according to claim 166 wherein the sensing member detects a level of engagement between the syringe holder and the medical injector system.
- 5 168 A sensing system according to claim 166 wherein the sensing member is a light sensor.
- 169 A sensing system according to claim 166 wherein the sensing member is a mechanical sensor.
- 10 170 A sensing system according to claim 166 wherein the sensing member is an electromagnetic sensor.
- 171 A sensing system according to claim 168 comprising a reflecting member to reflect light to the sensing member.
- 172 A sensing system according to claim 171 wherein the reflecting member is associated with a biasing member adapted to partially eject the syringe from the syringe holder upon release of a catch.
- 15 173 A sensing system according to claim 172 wherein the reflecting member is associated with the syringe.
- 174 A method for engaging a syringe holder according to claim 14 with a medical injector comprising the steps of;
- 20 (i) aligning the engaging portion of the syringe holder with a complimentary portion on the medical injector; and
- (ii) engaging the syringe holder with the medical injector.
- (iii) detecting a level of engagement between the syringe holder and the medical injector system.
- 25 175 A method for disengaging a syringe holder according to claim 14 from a medical injector comprising the steps of;

- (i) disengaging the engaging portion of the syringe holder from the medical injector; and
 - (ii) removing the syringe holder from the medical injector
 - (iii) detecting a level of disengagement between the syringe holder and the medical injector system.
- 5
- 176 A method for loading a syringe into a syringe holder of a medical injector system comprising a sensing system according to claim 166 comprising the steps of;
- (i) inserting the syringe barrel in a cradle of the syringe holder; and
 - (ii) sensing the presence of the syringe in the holder with a sensing member associated with the sensing system.
- 10
- 177 A method for removing a syringe, from a syringe holder of a medical injector system comprising a sensing system according to claim 166 comprising the steps of;
- (i) withdrawing the syringe from the cradle member; and
 - (ii) sensing the absence of a syringe in the holder with a sensing member associated with the sensing system.
- 15
- 178 A method for removing a syringe from a syringe holder according to claim 177 further comprising the step of automatically retracting the plunger after withdrawal of the syringe.
- 20
- 179 A method for removing a syringe from a syringe holder according to claim 177 further comprising the step of restricting retraction of the plunger until the syringe has been withdrawn.
- 180 A method for modifying a medical injector system comprising the steps of:
- (i) replacing the syringe holder with a syringe holder according to claim 42
 - (ii) attaching a plunger according to claim 74.
- 25
- 181 A method for modifying a medical injector system comprising the step of adding a sensing system according to claim 166.

- 182 A method for modifying a medical injector system comprising the step of adding a sensing system according to claim 157.
- 183 A medical injector system for injecting fluid from a syringe into a patient,
the syringe having a barrel and a hub slidably engaging the barrel
5 the hub comprising an inner surface having an engaging portion adapted to be releasably engaged by a plunger
the injector system comprising:
(i) a plunger for driving the hub, the plunger comprising a retention member adapted to releasably engage the engaging portion of the hub; and
10 (ii) a syringe holder comprising:
a cradle member adapted to receive a barrel of the syringe; and
a pivotable catch to releasably lock the syringe in the cradle member.
- 184 A medical injector system according to claim 183 further comprising a positioning device located on the cradle member to locate one end of the syringe in a
15 predetermined location in the cradle member.
- 185 A medical injector system according to claim 183 wherein the syringe holder comprises an engagement portion to enable simple releasable engagement with a medical injector.
- 186 A medical injector system according to claim 185 wherein the engagement portion
20 of the syringe holder comprises a locking member.
- 187 A medical injector system according to claim 185 wherein the locking member of the syringe holder comprises a slot.
- 188 A medical injector system according to claim 185 wherein the locking member of the syringe holder comprises a pin.
- 25 189 A medical injector system according to claim 183 further comprising:
(i) a tube adapted to be connected to syringe to conduct fluid into or out of the syringe; and
(ii) a connector to connect the tube to a vessel containing medical fluid and thereby enable withdrawal of the fluid from the vessel into the syringe

wherein the connector comprises a hollow spike to create an aperture through a bung in the vessel upon piercing of the bung by the spike.

190 A medical injector system according to claim 189 wherein the connector further comprises:

- 5 (i) a male luer portion having a locking collar; and
(ii) a disengagement portion to enable permanent disengagement of the spike from the male luer portion.

191 A medical injector system according to claim 190 wherein the disengagement portion comprises a frangible neck.

10 192 A medical injector system according to claim 189 wherein the spike comprises a barbed portion to resist removal of the spike from the vessel.

193 A medical injector system according to claim 183 further comprising a clamp between the tube and a male luer connector of the syringe, the clamp being moveable into a locking thread of the male luer connector thereby clamping the tube to the male luer connector.
15

194 A medical injector system according to claim 193 wherein the clamp comprises a gripping portion to increase the grip between it and the tube.

195 A medical injector system according to claim 193 wherein the clamp comprises a gripping portion to increase the grip between it and the connector.

20 196 A medical injector system according to claim 193 wherein the clamp comprises a gripping portion to increase the grip between it and the tube and connector.

197 A medical injector system according to claim 194 wherein the gripping portion is barbed.

25 198 A medical injector system according to claim 194 wherein the gripping portion comprises a ridge.

199 A medical injector system according to claim 194 wherein the gripping portion comprises a screw thread.

- 200 A medical injector system according to claim 193 wherein the clamp is tamper evident.
- 201 A medical injector system according to claim 183 comprising a base member and a sensor to detect orientation of the syringe holder with respect to the base member.
- 5 202 A medical injector system according to claim 201 wherein the sensor detects the angle between the syringe holder and base member.
- 203 A medical injector system according to claim 183 further comprising a switch to automatically initiate or inhibit movement of the plunger in the barrel depending on its orientation.
- 10 204 A medical injector system according to claim 203 wherein the switch is activated by a weight mechanism.
- 205 A medical injector system according to claim 183 further comprising a controller to control the movement of the plunger.
- 206 A medical injector system according to claim 205 comprising a base member and a sensor to detect orientation of the syringe holder with respect to the base member.
- 15 207 A medical injector system according to claim 206 wherein the sensor detects the angle between the syringe holder and base member.
- 208 A medical injector system according to claim 205 wherein the controller is operable to move the plunger to test patency of an intravascular catheter connected via a tube to the syringe.
- 20 209 A medical injector system according to claim 183 comprising a syringe holder according to claim 1.
- 210 A medical injector system according to claim 183 comprising a hub according to claim 43.
- 25 211 A medical injector system according to claim 183 comprising a plunger according to claim 74.
- 212 A medical injector system according to claim 183 comprising a plunger according to claim 109.

- 213 A medical injector system according to claim 183 comprising a sensor to detect a level of engagement between the plunger and the hub.
- 214 A medical injector system according to claim 213 wherein the sensor detects full engagement between the plunger and hub.
- 5 215 A medical injector system according to claim 213 comprising a light sensor.
- 216 A medical injector system according to claim 215 wherein the light sensor comprises a fibre optic cable.
- 217 A medical injector system according to claim 213 comprising a mechanical sensor.
- 218 A medical injector system according to claim 213 comprising an electromagnetic
10 sensor.
- 219 A medical injector system according to claim 205 comprising a sensor to detect a level of engagement between the plunger and the hub.
- 220 A medical injector system according to claim 219 wherein the sensor communicates with the controller to further control the movement of the plunger.
- 15 221 A medical injector system according to claim 220 wherein the communication enables engagement of the plunger and the hub without thereby moving the hub.
- 222 A medical injector system according to claim 220 wherein the communication enables releasable locking of the hub to the plunger.
- 223 A medical injector system according to claim 220 wherein the communication
20 causes releasable locking of the hub to the plunger.
- 224 A medical injector system according to claim 220 wherein the communication enables detection of used syringes.
- 225 A medical injector system according to claim 224 wherein a signal is created if the sensor detects the hub at a position forward of its most retracted state.
- 25 226 A medical injector system according to claim 220 wherein the communication enables detection of errors.

- 227 A medical injector system according to claim 226 wherein a signal is created if the hub and plunger disengage prematurely.
- 228 A medical injector system according to claim 183 adapted for use with a device according to any one of claims 136.
- 5 229 A medical injector system according to claim 183 comprising the sensing system of claim 157.
- 230 A medical injector system according to claim 183 comprising the sensing system of claim 166.
- 231 A medical injector system according to claim 205 comprising the syringe sensing system of claim 157.
- 10 232 A medical injector system according to claim 205 comprising the syringe sensing system of claim 166.
- 233 A medical injector system according to claim 205 comprising the sensing system of claim 167.
- 15 234 A medical injector system according to claim 232 wherein the sensing member communicates with the controller to modify operation of the injector system.
- 235 A medical injector system according to claim 234 wherein the communication enables movement of the plunger to either fill or expel fluid from the syringe.
- 236 A medical injector system according to claim 234 wherein the communication disables movement of the plunger.
- 20 237 A medical injector system according to claim 234 wherein movement of the plunger is disabled after use if the syringe has not been removed.
- 238 A medical injector system according to claim 234 wherein movement of the plunger is disabled before use if the syringe has not been engaged to a specified level.
- 25 239 A medical injector system according to claim 234 wherein movement of the plunger is disabled before use if the syringe holder has not been engaged to a specified level.

- 240 A medical injector system according to claim 234 wherein a signal is created if removal of the syringe is attempted at certain orientations of the syringe.
- 241 A medical injector system according to claim 240 wherein the signal is created if removal is attempted while the syringe is in a substantially vertical orientation.
- 5 242 A syringe for use with a medical injector system comprising a plunger according to claim 74 and a hub according to claim 43.
- 243 A medical injector system according to claim 183 comprising a syringe according to claim 154.
- 244 A medical injector system according to claim 183 comprising a syringe according to claim 155.
- 10
- 245 A method of filling a syringe with medical fluid from a sealed vessel the syringe for use with a medical injector system comprising the steps of:
- (i) elevating the front portion of the syringe relative to the back portion;
 - (ii) advancing a plunger to a position within the syringe corresponding to a predetermined patient dose;
 - 15 (iii) controlling movement of the plunger in a sequence of forward and backward movements to expel air from the syringe and any attached tube into the vessel bottle, and draw the desired dose of fluid into the syringe.
- 246 A method of filling a syringe according to claim 245 further comprising the step of automatically restricting the direction of movement of the plunger depending on the orientation of the syringe.
- 20
- 247 A method of filling a syringe according to claim 245 wherein the plunger may move either forward or backward when oriented with its front portion elevated with respect to its back portion and only in the forward direction when oriented with the back portion elevated with respect to its front portion.
- 25
- 248 A method of filling a syringe with medical fluid from a sealed vessel the syringe for use with a medical injector system according to claim 183, comprising the steps of:
- (i) elevating the front portion of the syringe relative to the back portion;
 - (ii) advancing the plunger to a position within the syringe corresponding to a

predetermined patient dose;

(iii) controlling movement of the plunger in a sequence of forward and backward movements to expel air from the syringe and any attached tube into the vessel bottle, and draw the desired dose of fluid into the syringe.

- 5 249 A method of filling a syringe according to claim 248 further comprising the step of automatically restricting the direction of movement of the plunger depending on the orientation of the syringe.
- 250 A method of filling a syringe according to claim 248 wherein the plunger may move either forward or backward when oriented with its front portion elevated with respect to its back portion and only in the forward direction when oriented with the
10 back portion elevated with respect to its front portion.
- 251 A method of injecting a patient using a medical injector system according to claim 183 comprising the steps of;
- 15 (i) engaging the plunger with the hub;
- (ii) driving the hub along the syringe barrel; and
- (iii) expelling fluid from the syringe into a patient.
- 252 A method for engaging a syringe holder according to claim 14 with a medical injector according to claim 183, comprising the steps of;
- 20 (i) aligning the engaging portion of the syringe holder with a complimentary portion on the medical injector; and
- (ii) engaging the syringe holder with the medical injector.
- 253 A method for engaging a syringe holder according to claim 252 comprising the further step of detecting a level of engagement between the syringe holder and the medical injector system.
- 25 254 A method for disengaging a syringe holder according to claim 14 from a medical injector according to claim 183, comprising the steps of;
- (i) disengaging the engaging portion of the syringe holder from the medical injector; and

- (ii) removing the syringe holder from the medical injector.
- 255 A method for disengaging a syringe holder according to claim 254 comprising the further step of detecting a level of disengagement between the syringe holder and the medical injector system.
- 5 256 A method for loading a syringe into a syringe holder associated with a medical injector system according to claim 183, comprising the steps of;
- (i) inserting the syringe barrel in the cradle member such that the catch is displaced; and
 - (ii) allowing the catch mechanism to return into its biased position to engage the
- 10 syringe and thereby retain the syringe in the cradle member.
- 257 A method for removing a syringe, from a syringe holder associated with a medical injector system according to claim 183 comprising the steps of;
- (i) releasing the catch to unlock the syringe; and
 - (ii) withdrawing the syringe from the cradle member.
- 15 258 A method for loading a syringe into a syringe holder of a medical injector system according to claim 183 comprising the steps of;
- (i) inserting the syringe barrel in a cradle of the syringe holder; and
 - (ii) sensing the presence of the syringe in the holder with a sensing member associated with the sensing system.
- 20 259 A method for removing a syringe, from a syringe holder of a medical injector system according to claim 183 comprising the steps of;
- (i) withdrawing the syringe from the cradle member; and
 - (ii) sensing the absence of a syringe in the holder with a sensing member associated with the sensing system.
- 25 260 A method for removing a syringe from a syringe holder according to claim 259 further comprising the step of automatically retracting the plunger after withdrawal of the syringe.

- 261 A method for removing a syringe from a syringe holder according to claim 259 further comprising the step of restricting retraction of the plunger until the syringe has been withdrawn.
- 5 262 A method for removing a syringe from a syringe holder according to claim 259 further comprising the step of prompting retraction of the plunger after the syringe has been withdrawn.
- 263 A method of connecting a syringe hub to a plunger using a medical injector system according to claim 183 comprising the steps of;
- 10 (i) introducing the plunger into a syringe barrel within which the hub is slidably engaged and engaging the plunger with the inner surface of the hub; and
- (ii) activating the plunger such that a retention member engages the engaging portion of the hub.
- 15 264 A method of connecting a syringe hub to a plunger according to claim 263 further comprising the step of detecting a level of engagement between the plunger and the hub.
- 265 A method for modifying a medical injector system comprising a syringe holder, comprising the steps of:
- 20 (i) replacing the syringe holder with a syringe holder according to claim 1
- (ii) attaching a plunger according to claim 74.
- 266 A method for modifying a medical injector system comprising a syringe holder, comprising the steps of:
- (i) replacing the syringe holder with a syringe holder according to claim 1
- (ii) attaching a plunger according to claim 109.
- 25 267 A method for modifying a medical injector system comprising the steps of:
- (i) replacing the syringe holder with a syringe holder according to claim 41
- (ii) attaching a plunger according to claim 74.

- 268 A method for modifying a medical injector system comprising the steps of:
(i) replacing the syringe holder with a syringe holder according to claim 42
(ii) attaching a plunger according to claim 74.
- 269 A method for modifying a medical injector system comprising the step of adding a
5 sensing system according to claim 157.
- 270 A method for modifying a medical injector system comprising the step of adding a
sensing system according to claim 166.
- 271 A syringe holder for a medical injector system substantially as herein described
with reference to Figures 2, 18a to 18e, 20 to 23f and 36 to 42.
- 10 272 A hub for a syringe for use with a medical injector system substantially as herein
described with reference to Figures 2 to 17, 18d, 18e, 19 to 23a, 24, 28, 37b and 38
to 42
- 273 A plunger for a syringe for use with a medical injector system substantially as
herein described with reference to Figures 2c, 3 to 17, 19 to 23a, 37b and 38 to 40.
- 15 274 A device for manually filling a syringe for use with a medical injector system
substantially as herein described with reference to Figures 2c, 3 to 17, 19 to 23a,
37b and 38 to 40.
- 275 A syringe for use with a medical injector system substantially as herein described
with reference to Figures 2, 18d, 18e, 19 to 24, 28 to 33, 36 to 37b and 38 to 42.
- 20 276 A sensing system for use with a medical injector system substantially as herein
described with reference to Figures 36 to 42.
- 277 A medical injector system substantially as herein described with reference to
Figures 2 to 42

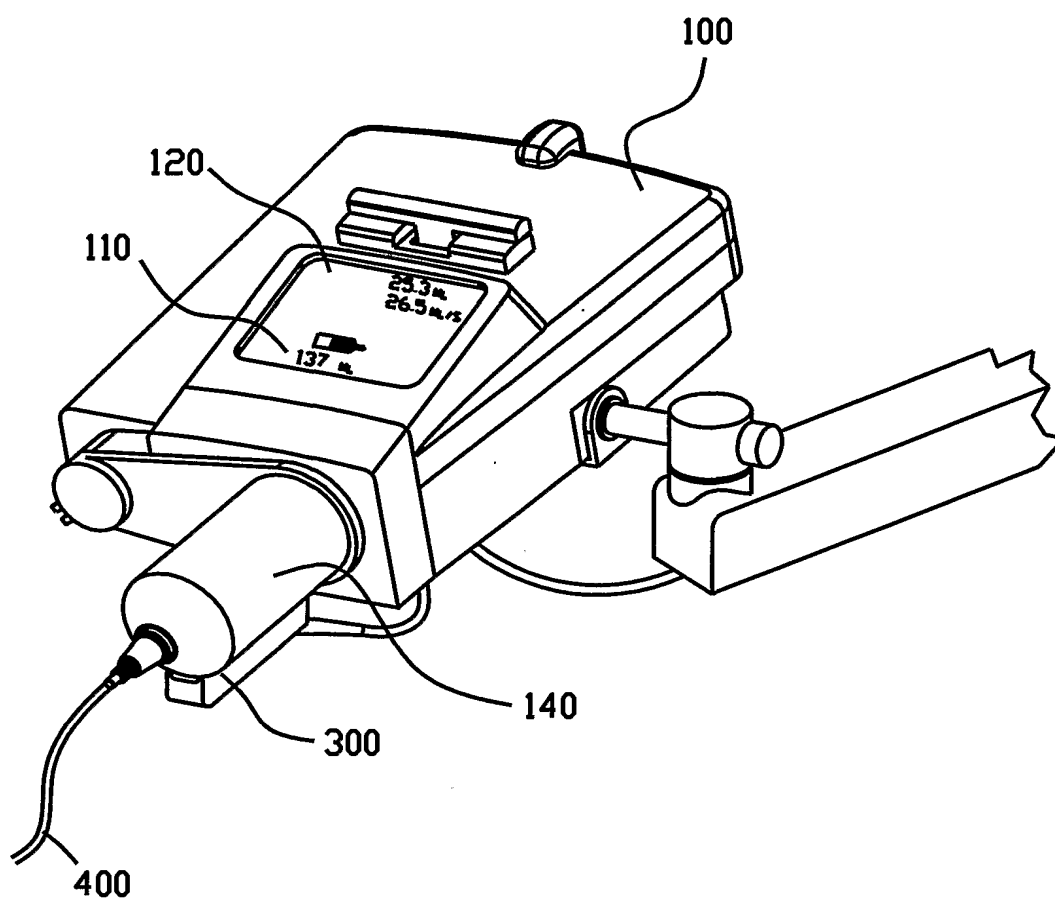


FIG. 1

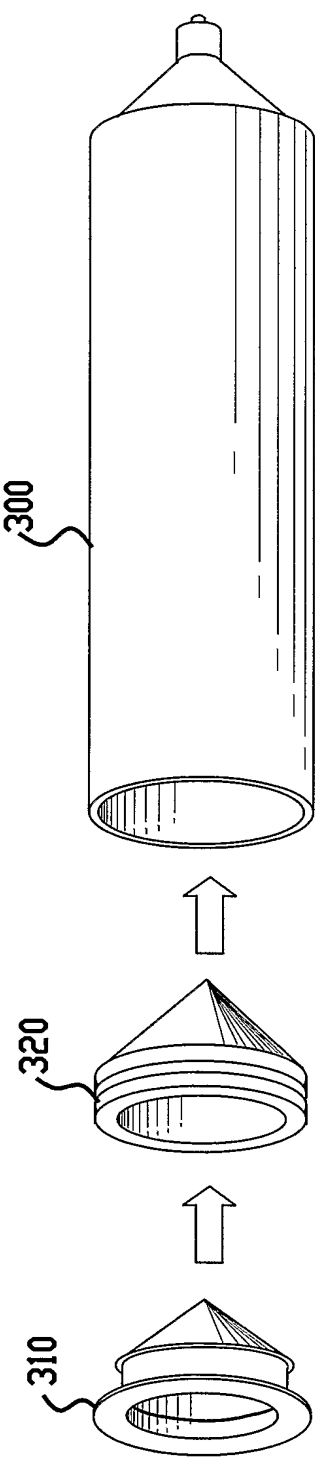


FIG. 2a

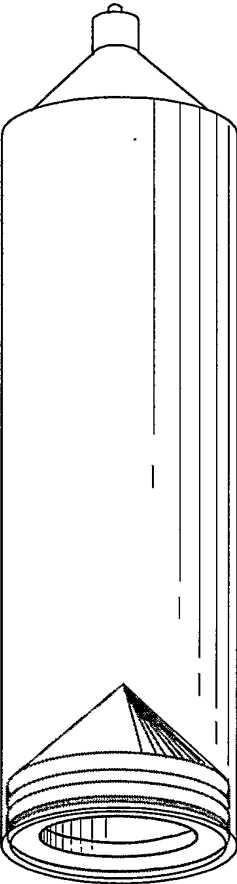


FIG. 2b

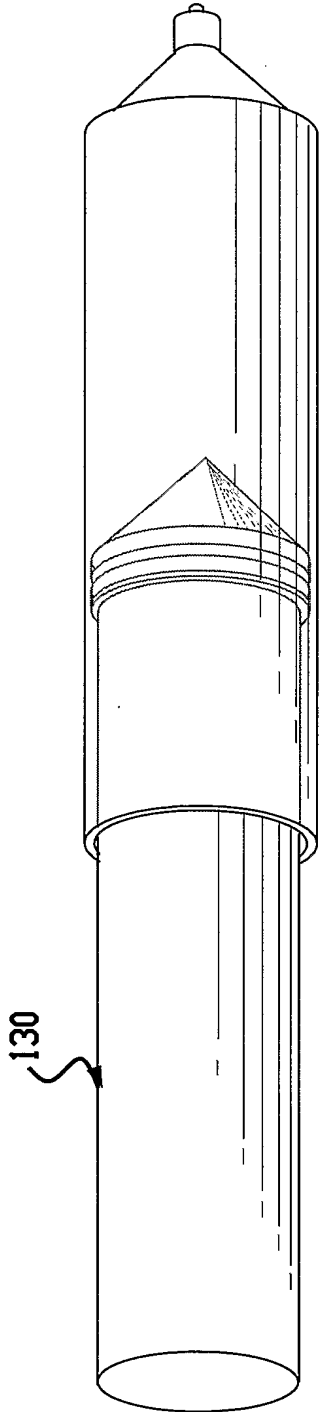


FIG. 2c

FIG. 2

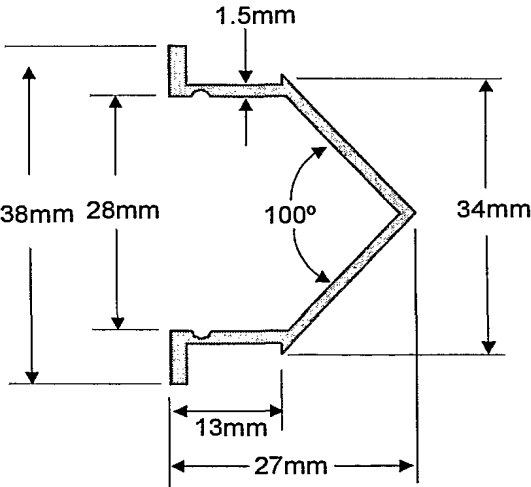
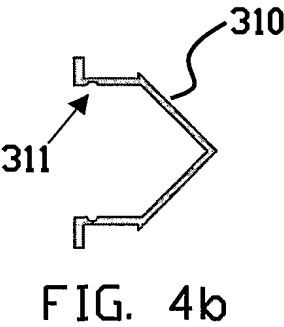
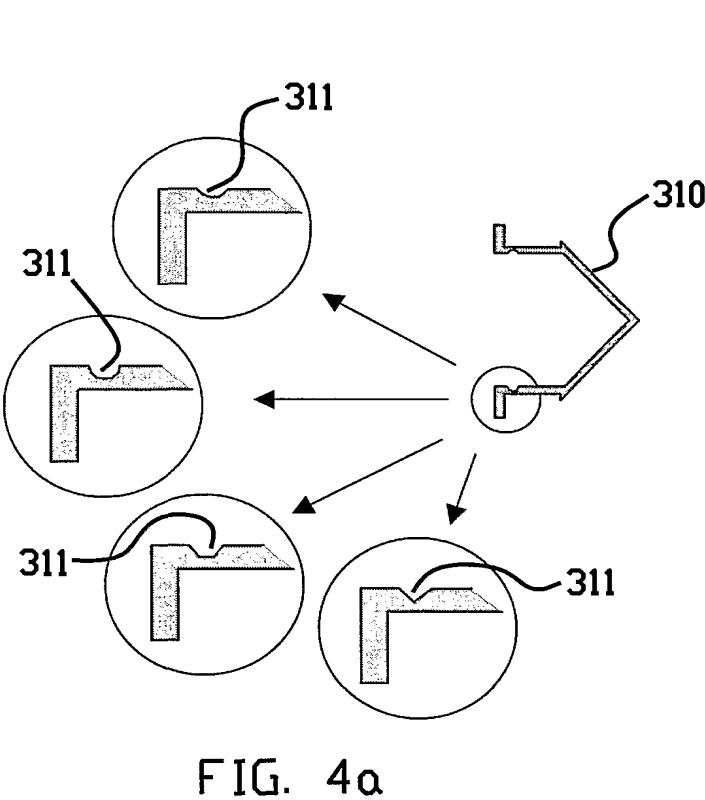
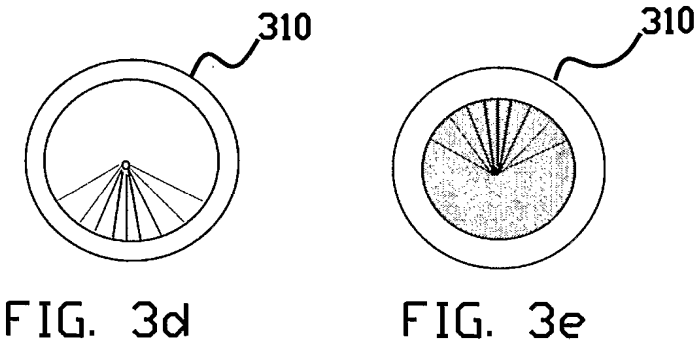
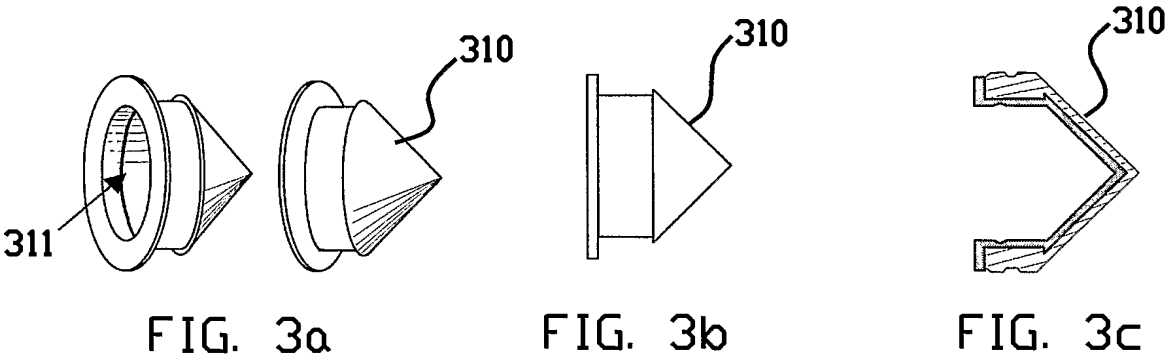


FIG. 5




FIG. 4c




FIG. 4d




FIG. 4e

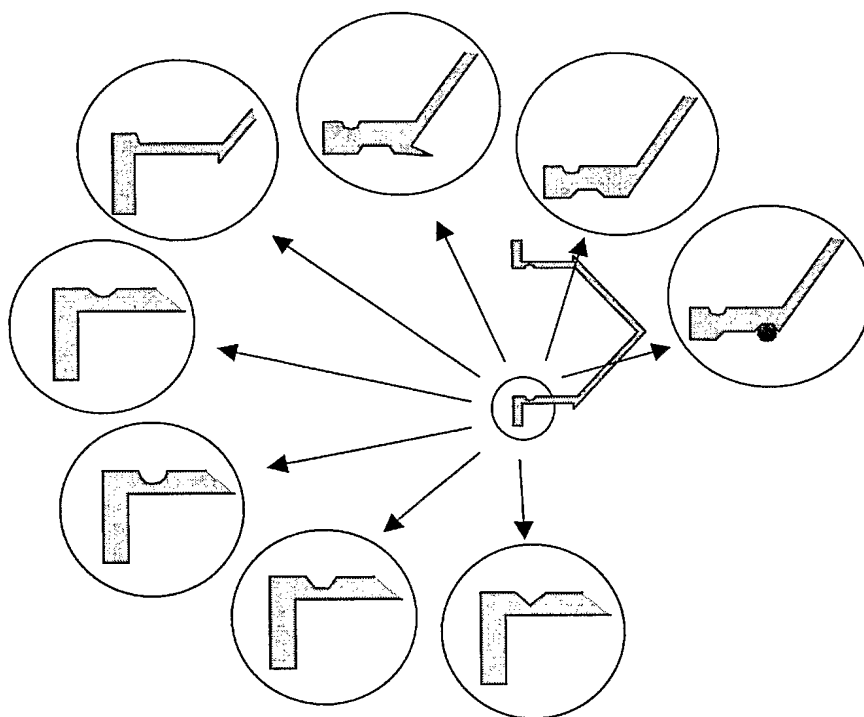


FIG. 4f

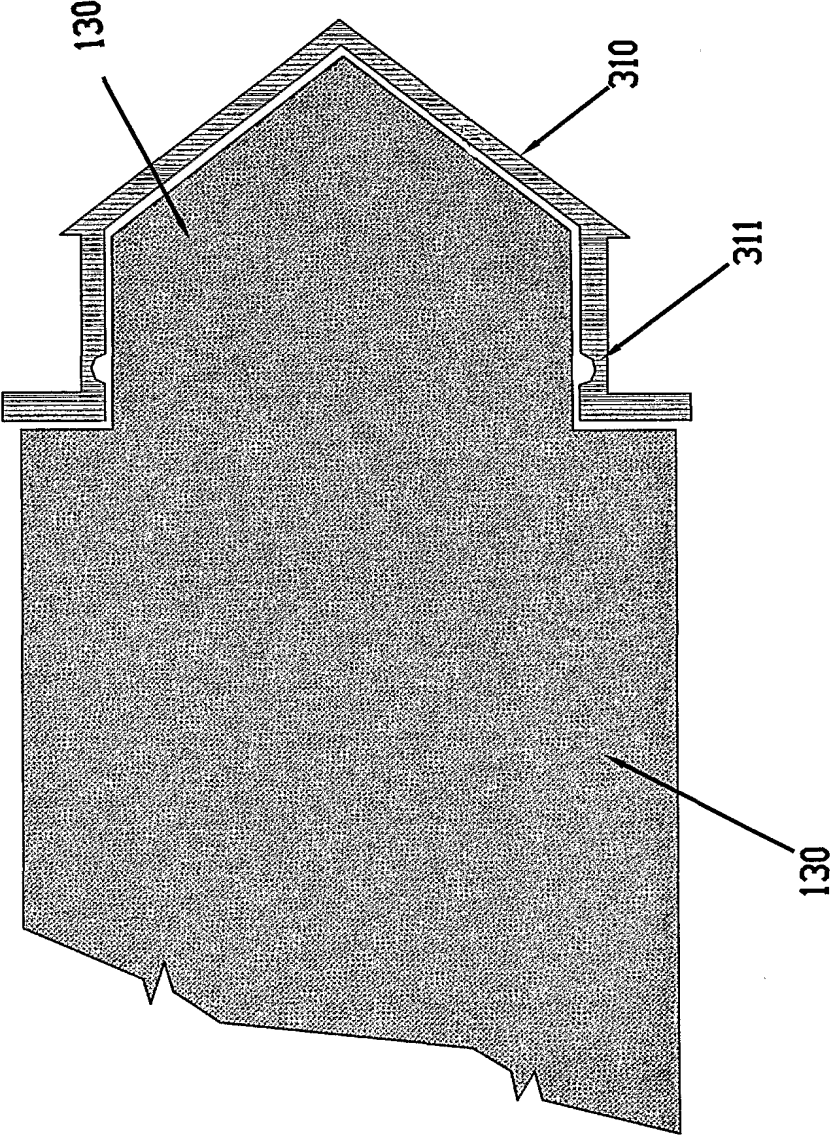
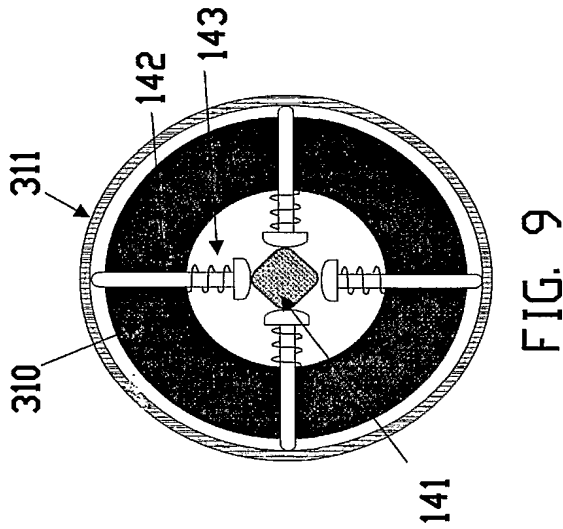
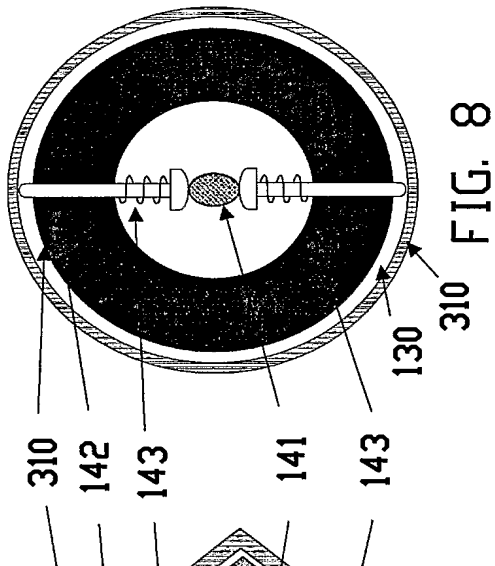
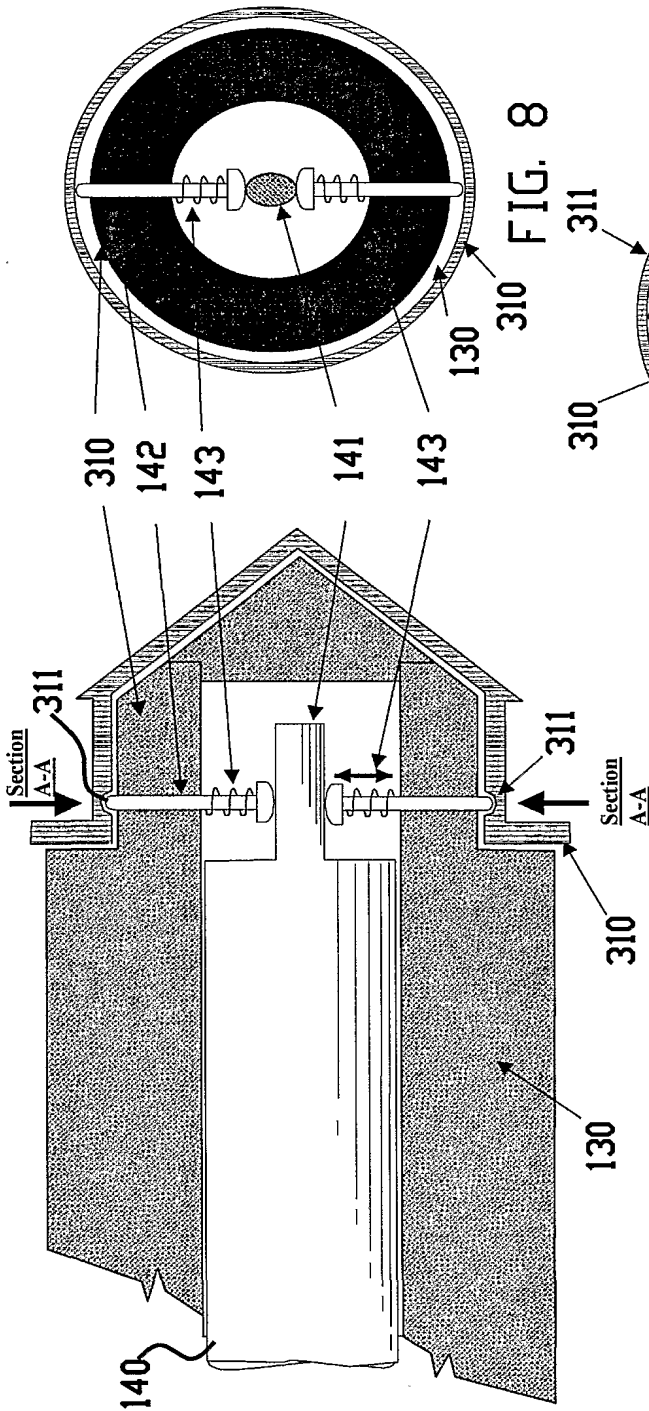


FIG. 6



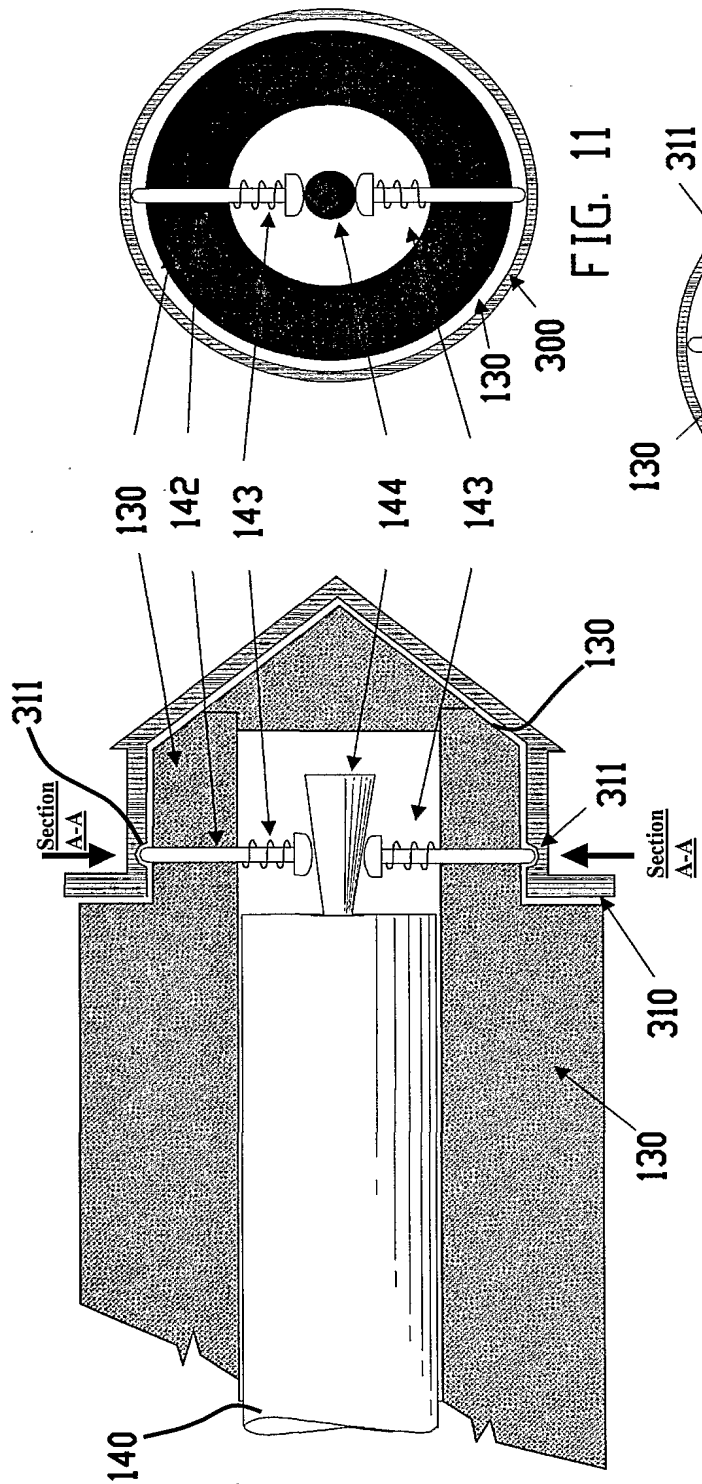


FIG. 10

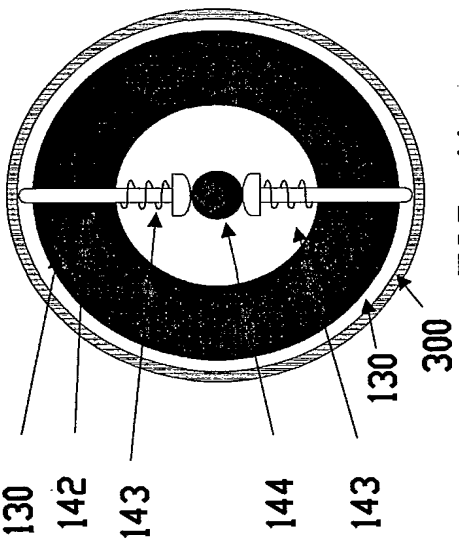


FIG. 11

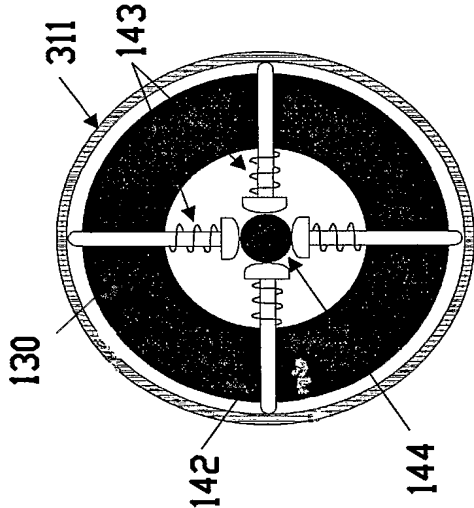
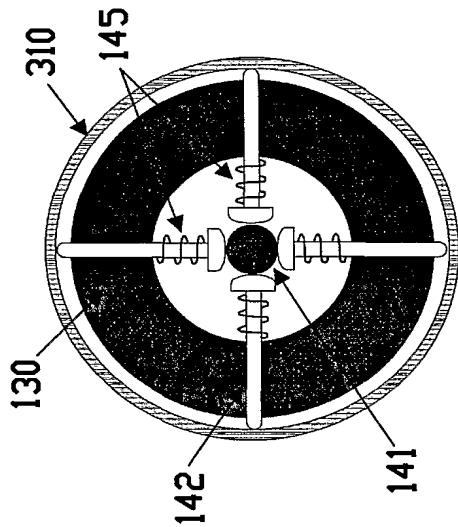
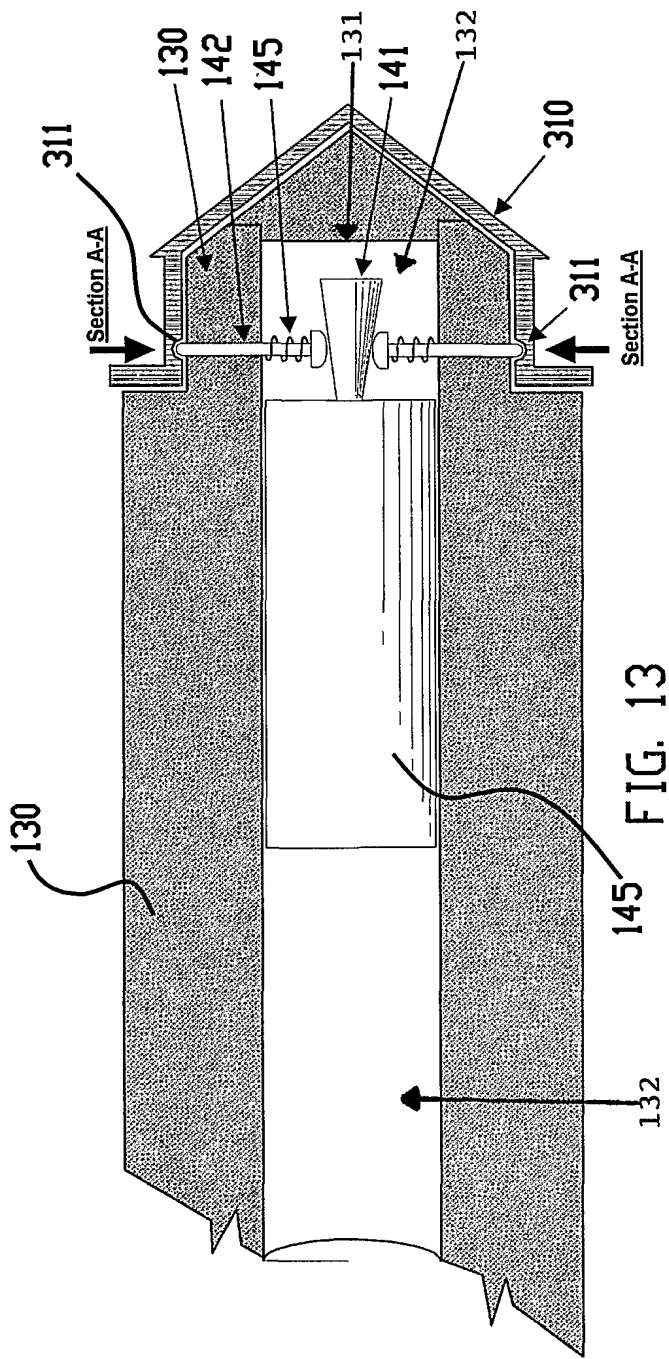
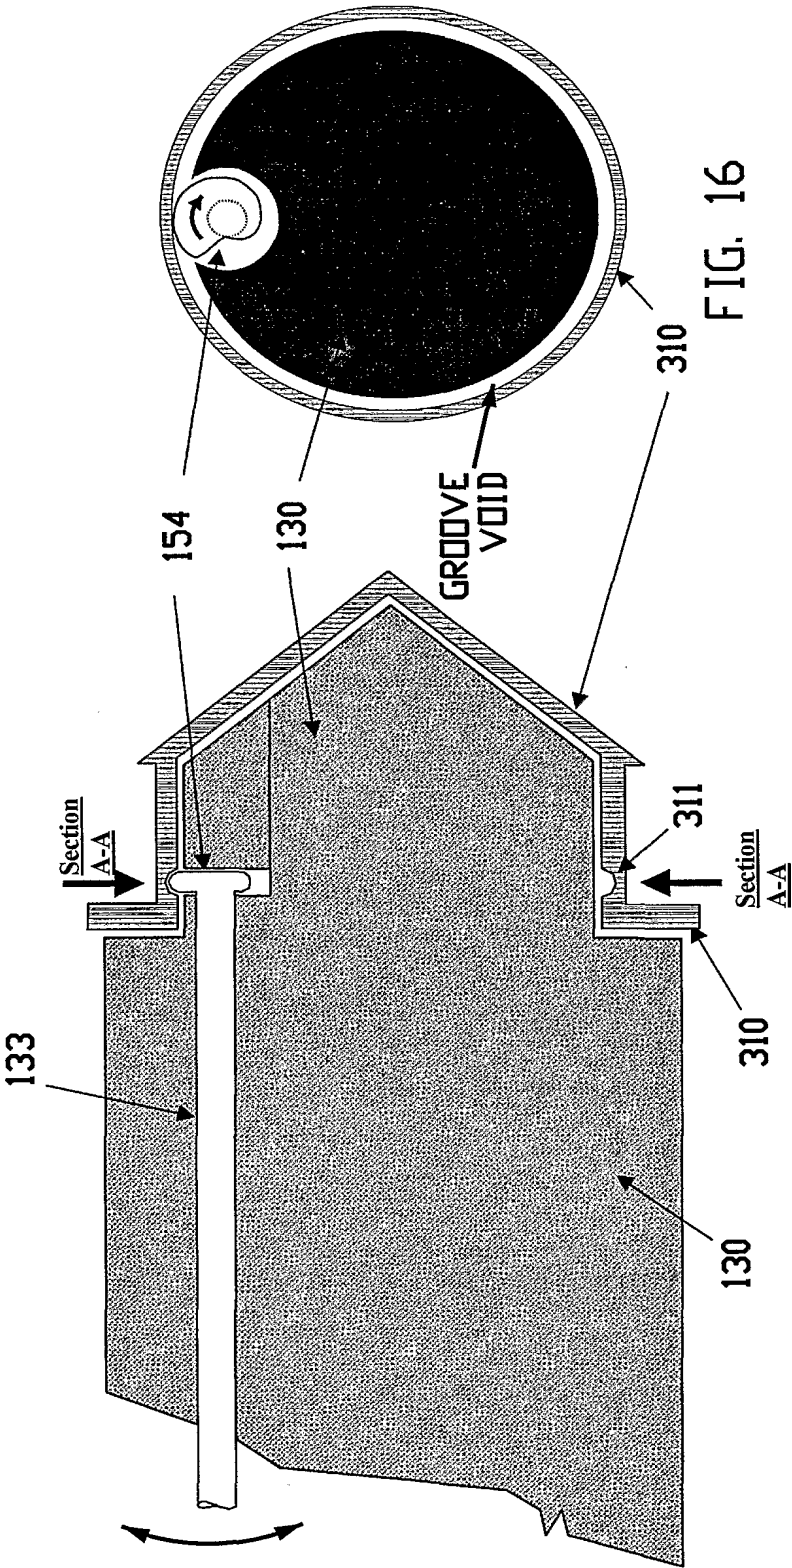


FIG. 12





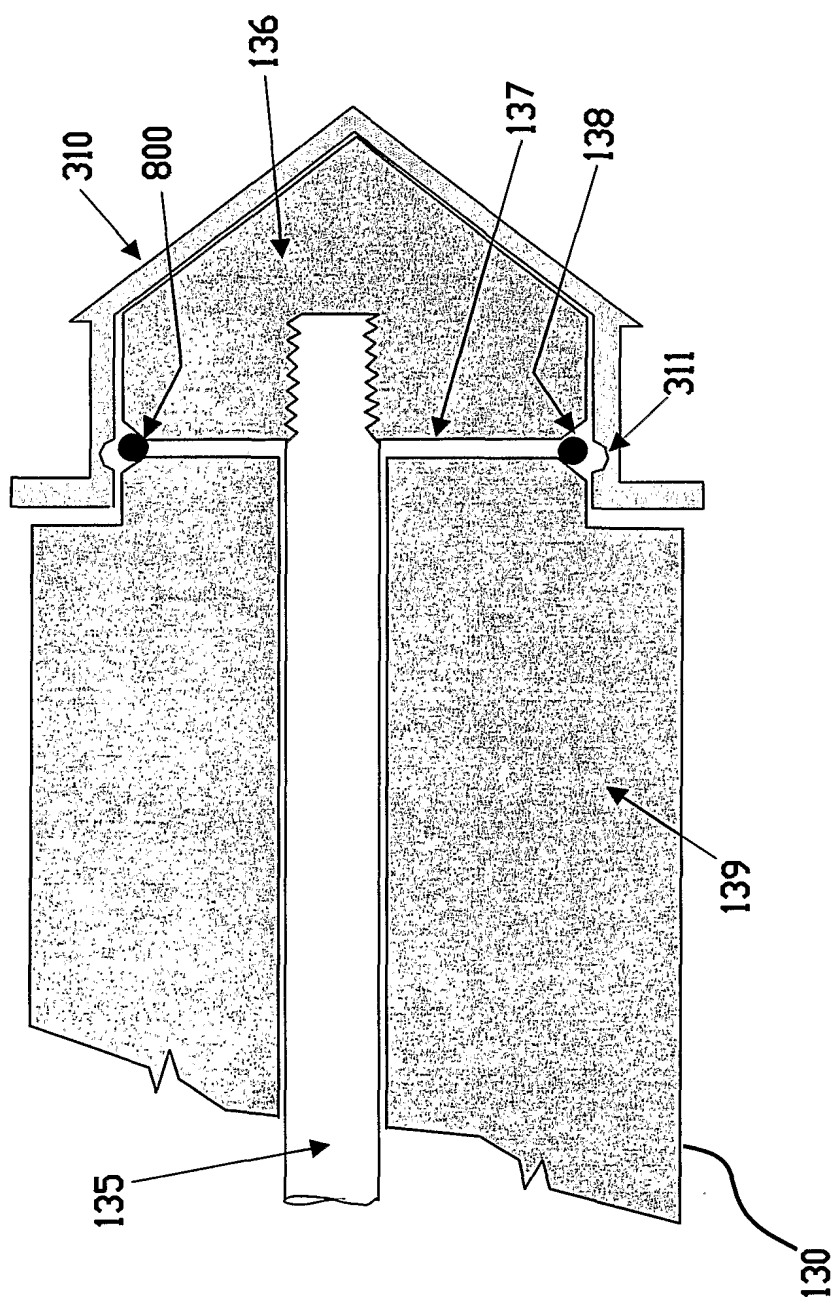


FIG. 17

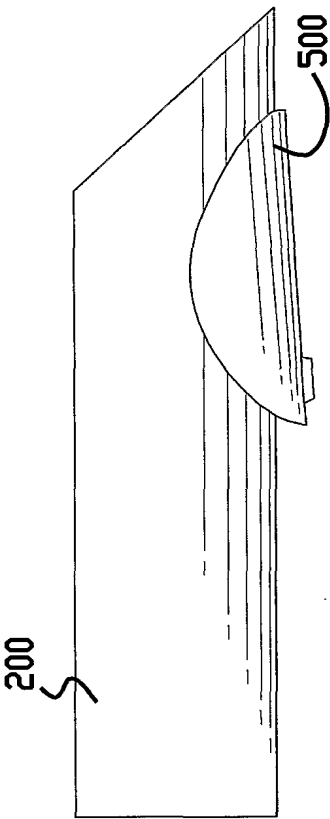


FIG. 18a

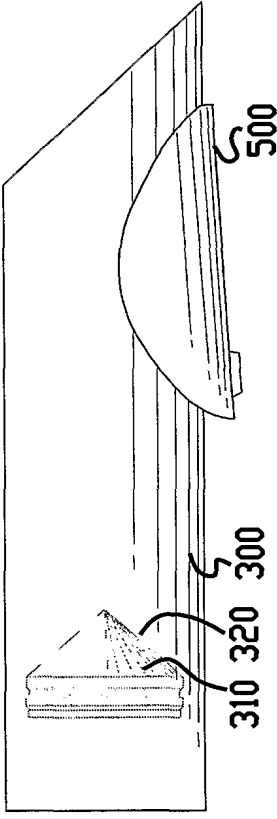


FIG. 18b

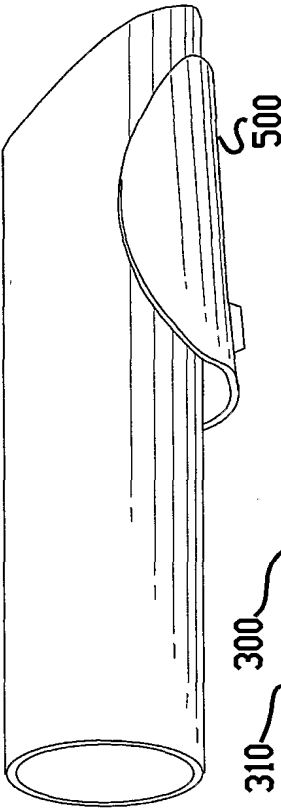


FIG. 18c

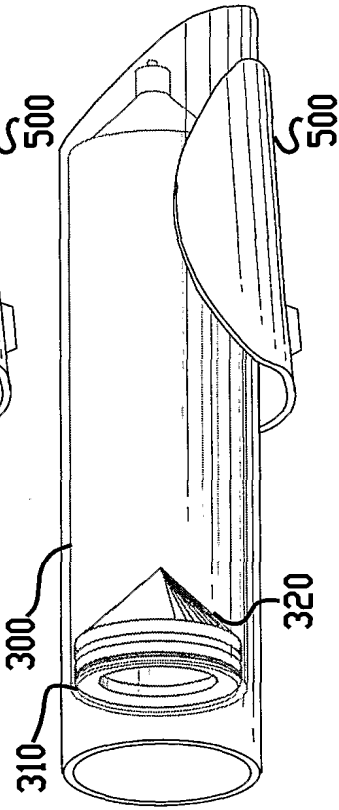
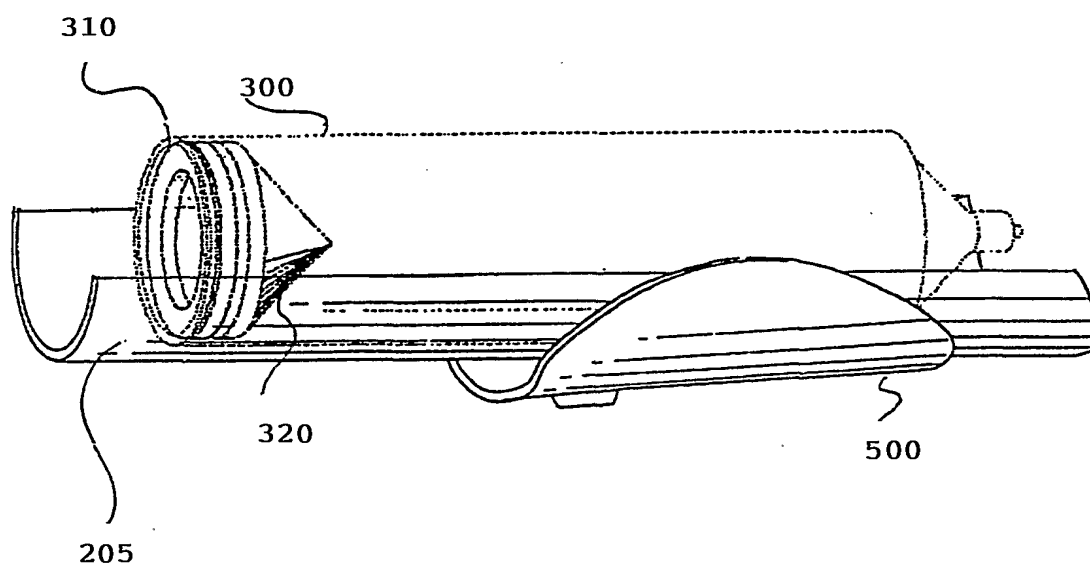


FIG. 18d

FIG. 18e



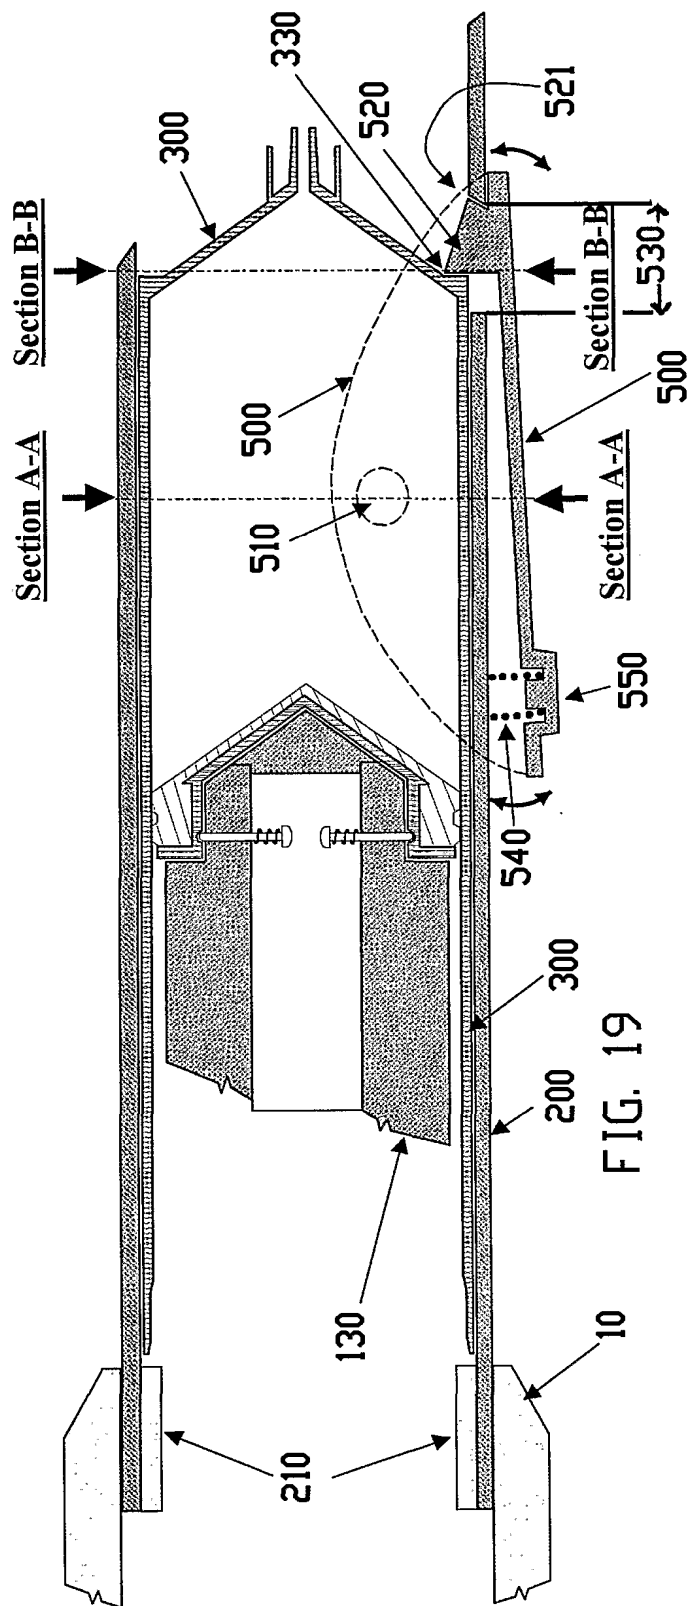


FIG. 19

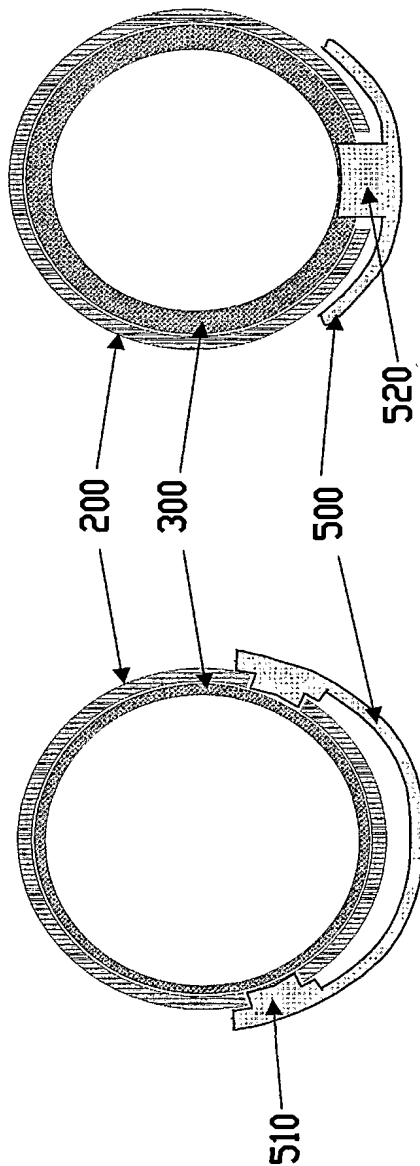


FIG. 20

FIG. 21

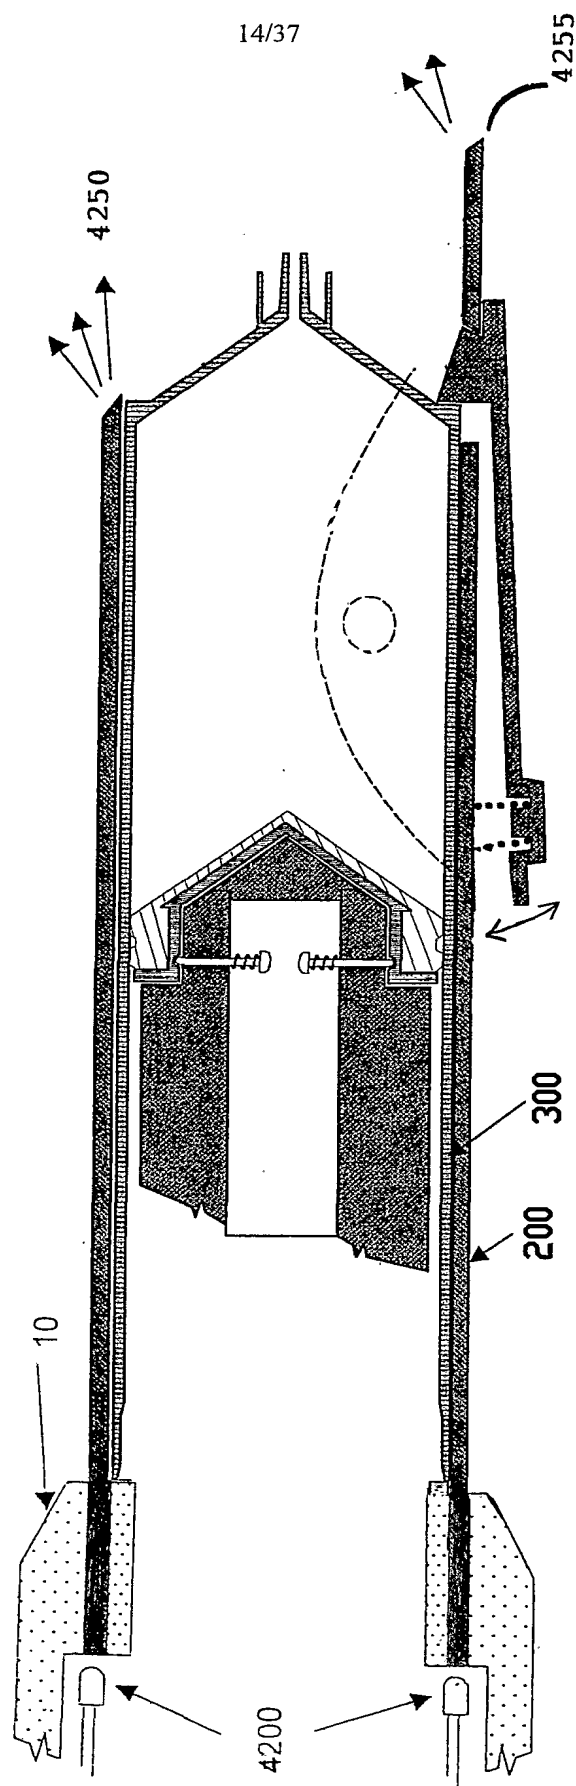


FIG. 22a

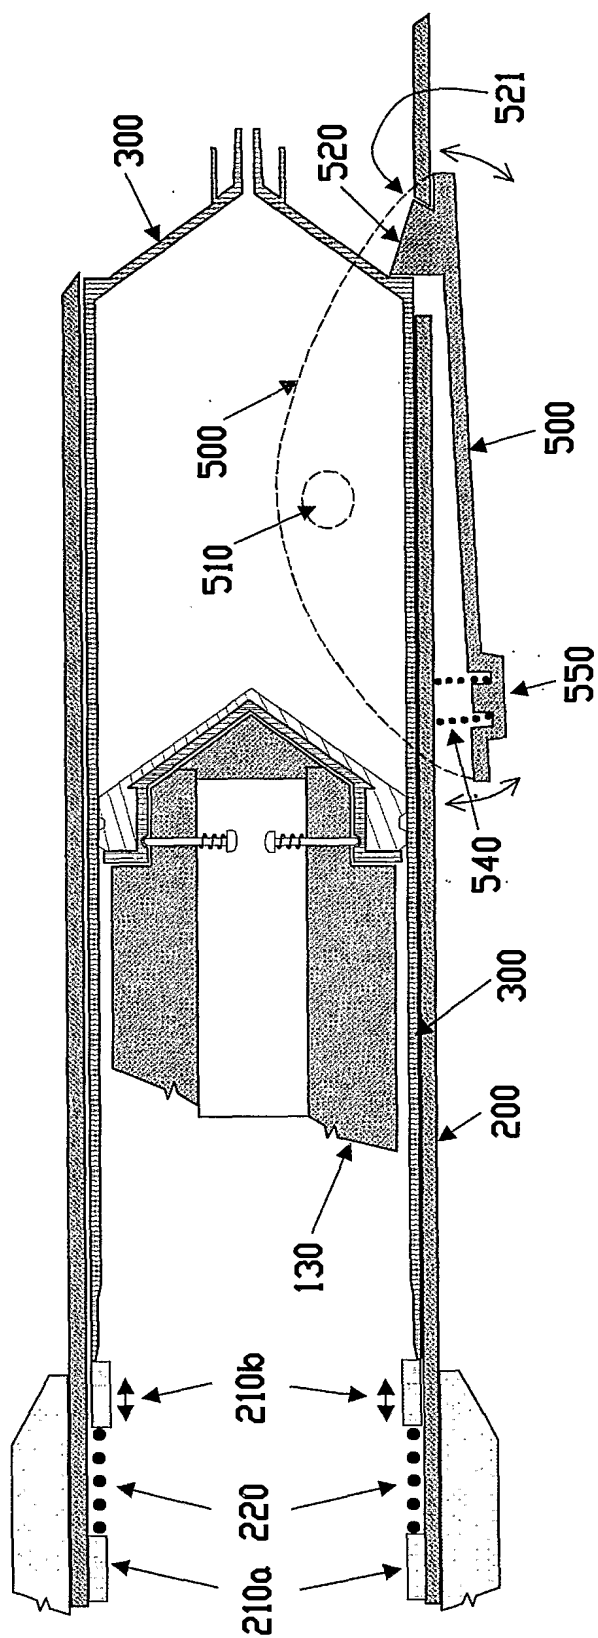


FIG. 22b

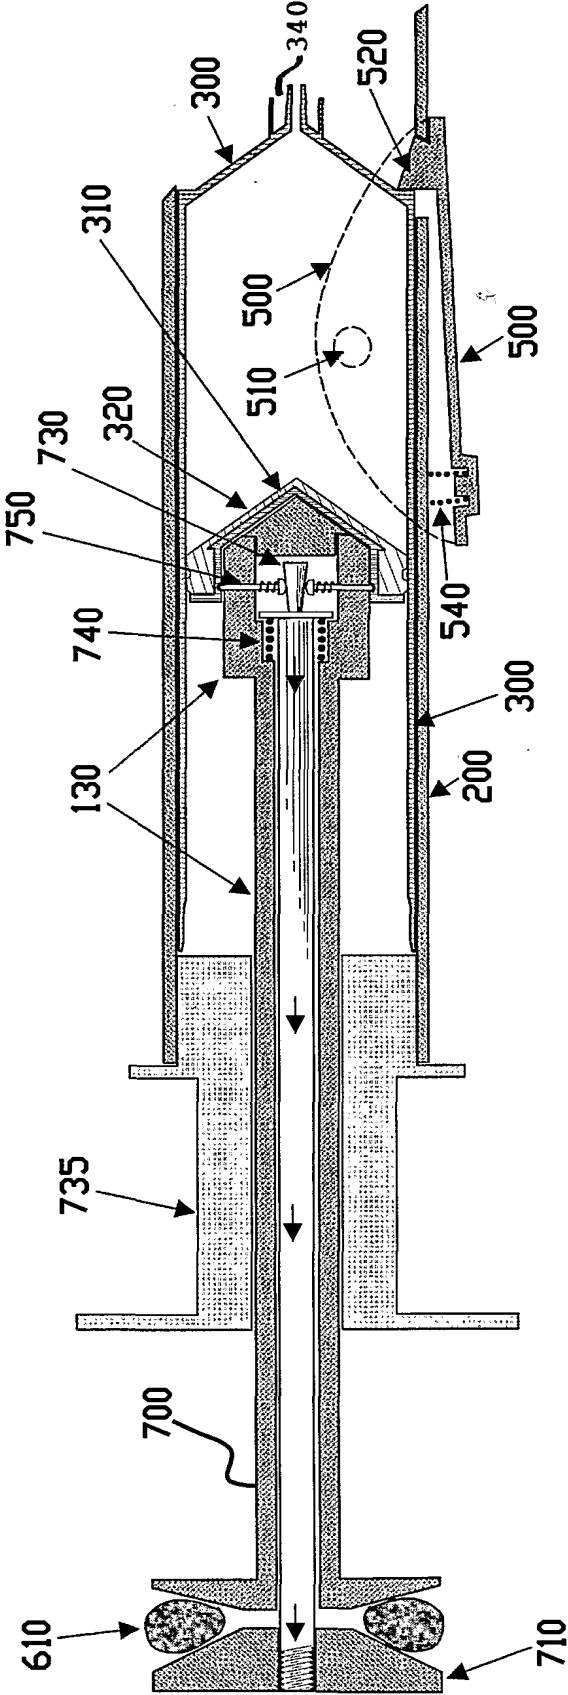


FIG. 23a

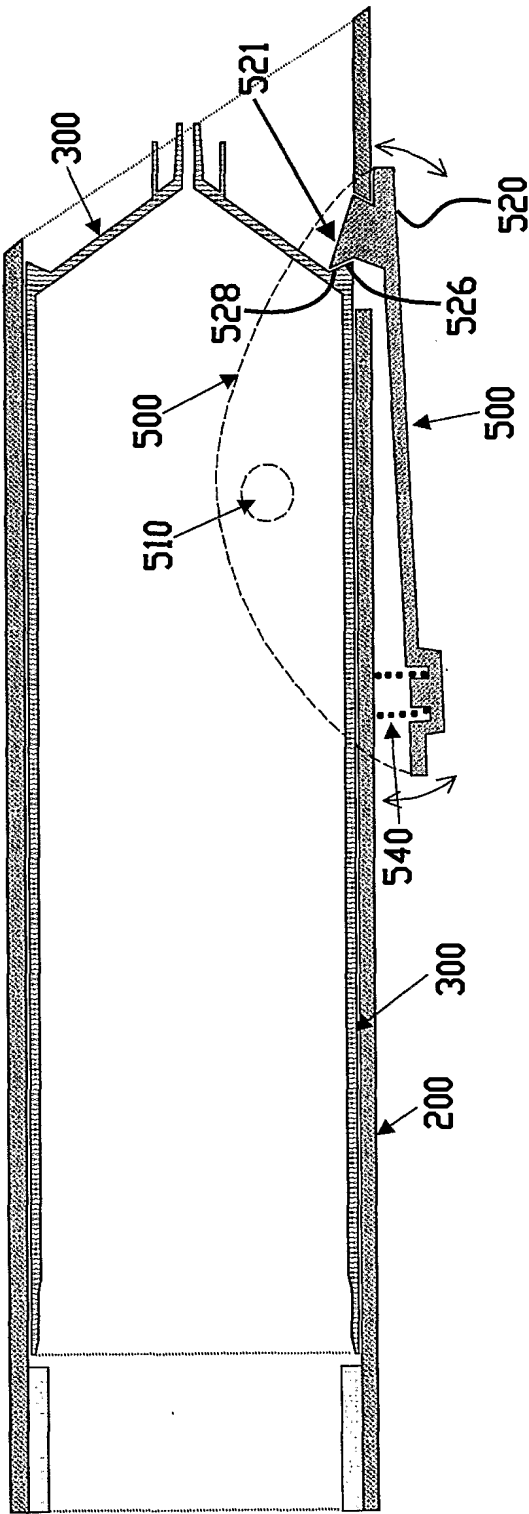


FIG. 23b

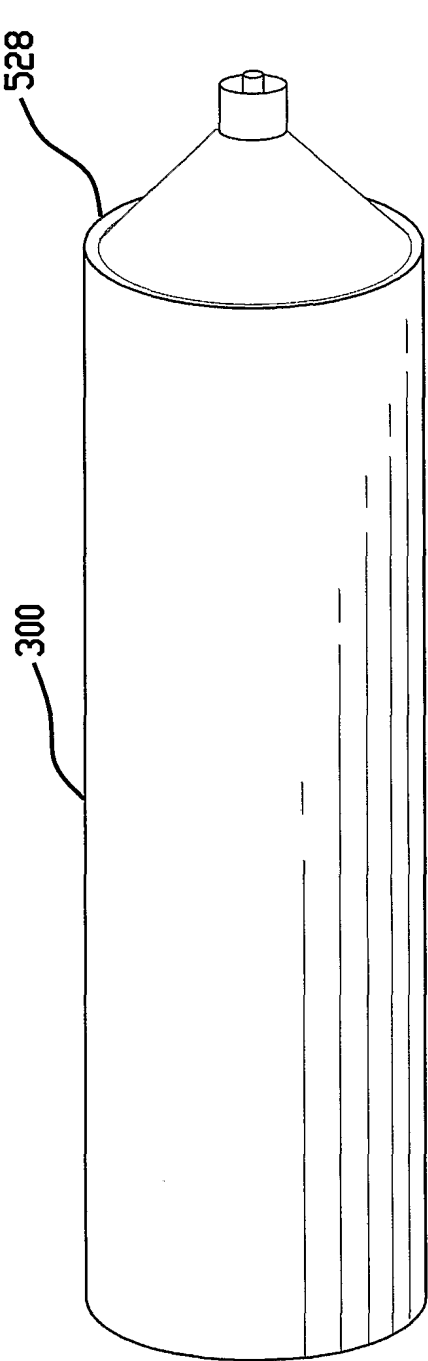


FIG. 23c

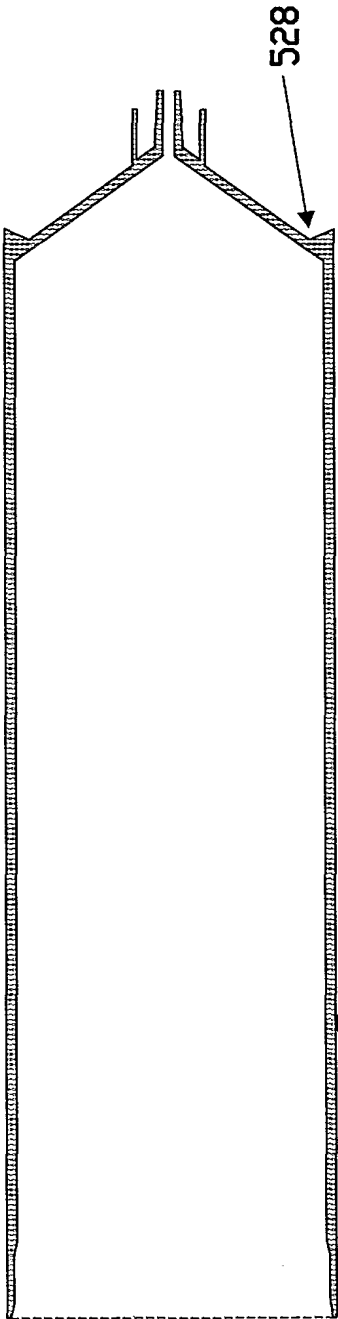


FIG. 23d

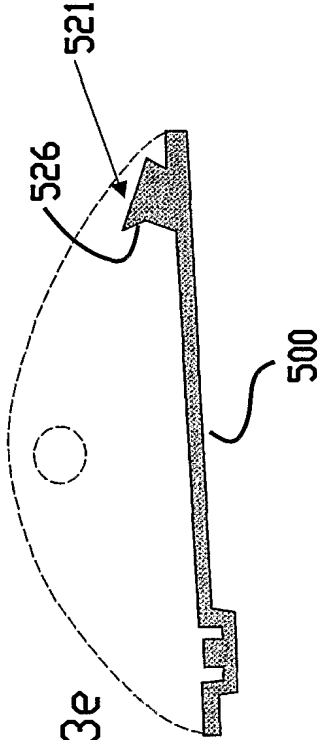


FIG. 23e

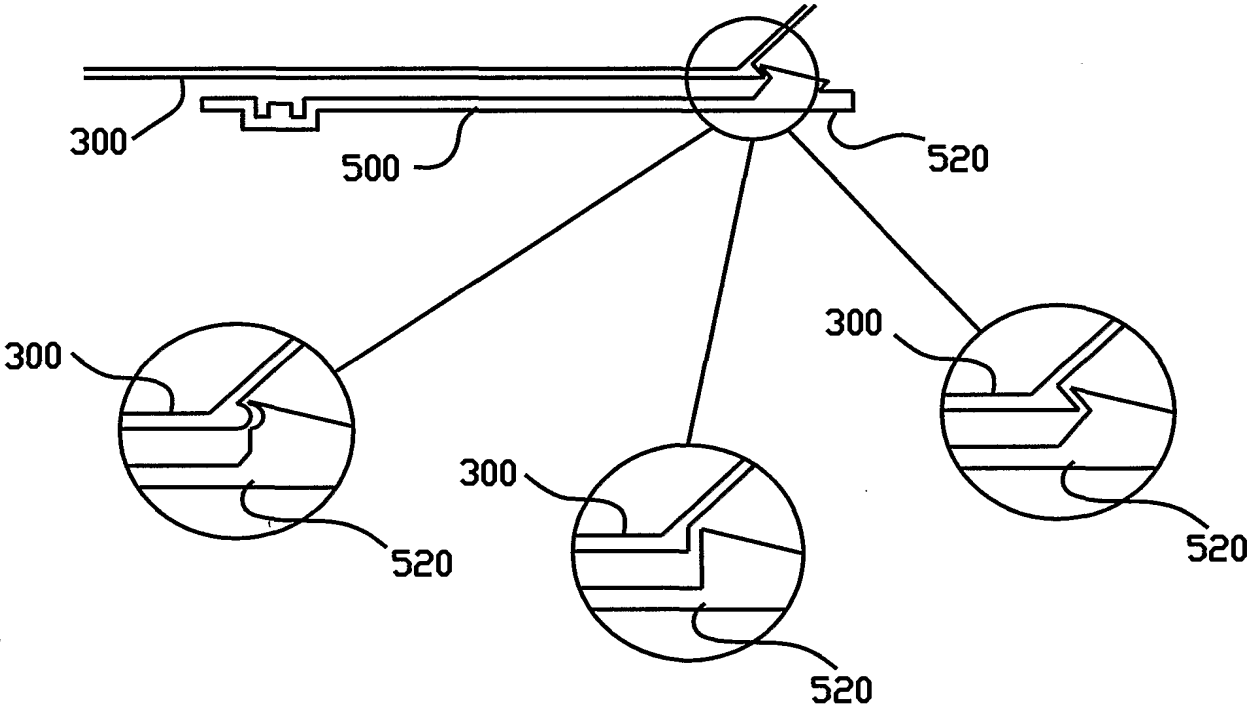


FIG. 23f

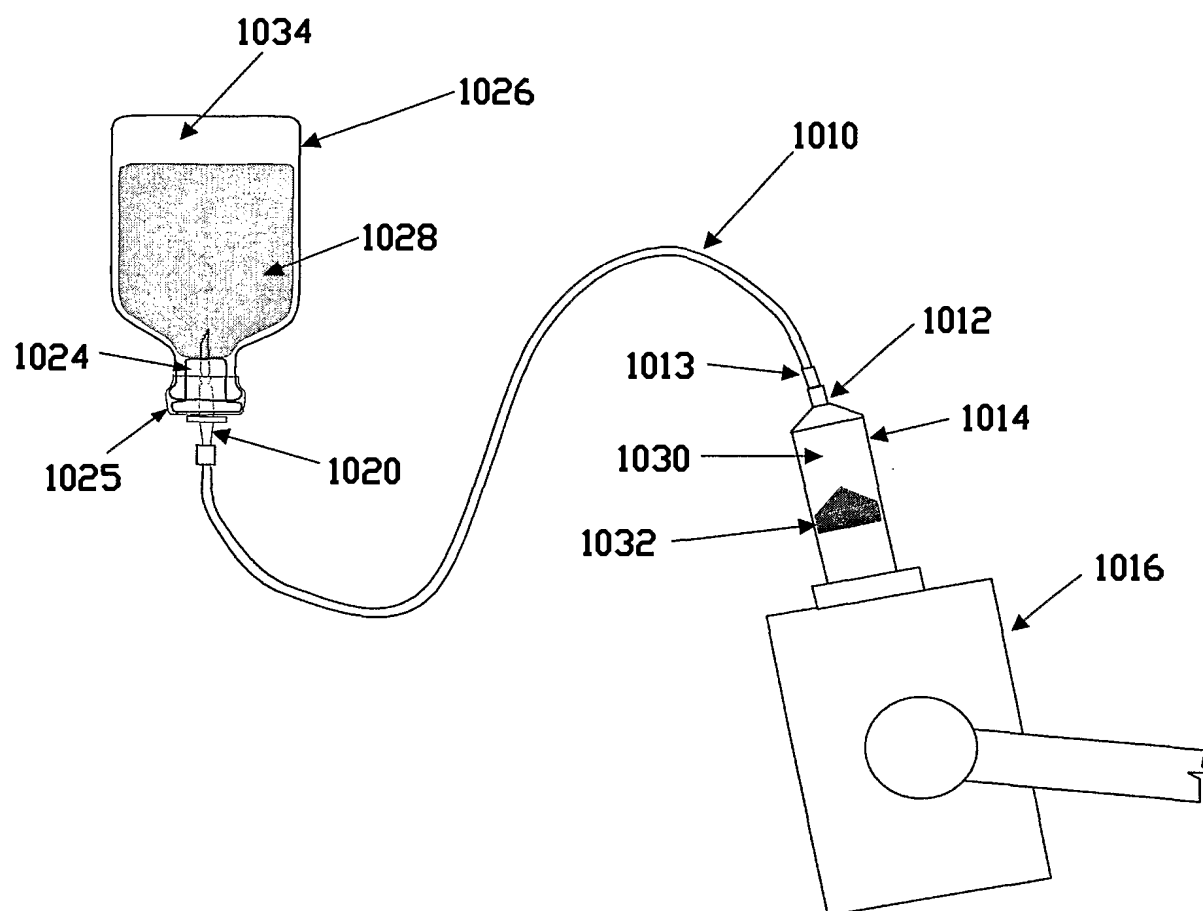


FIG. 24

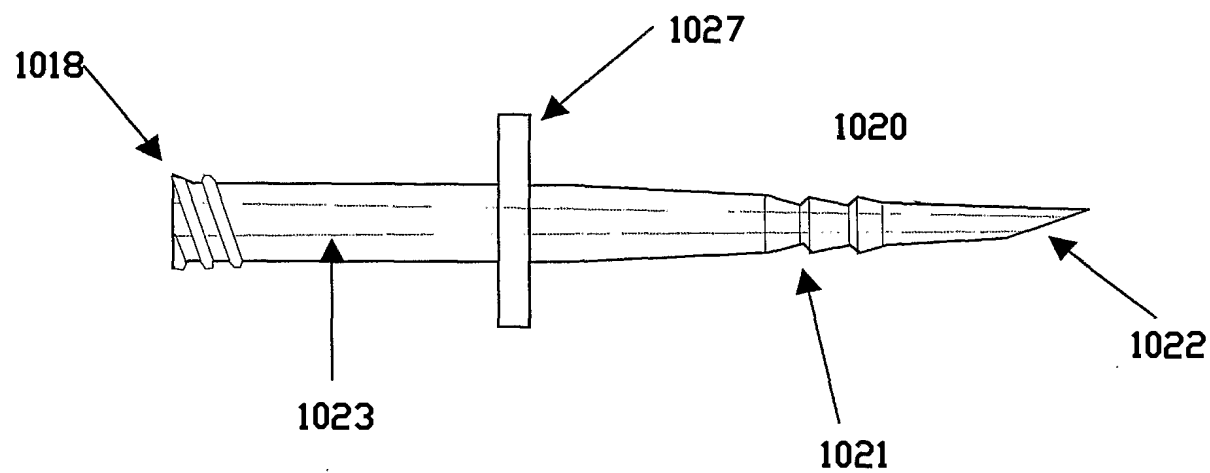


FIG. 25

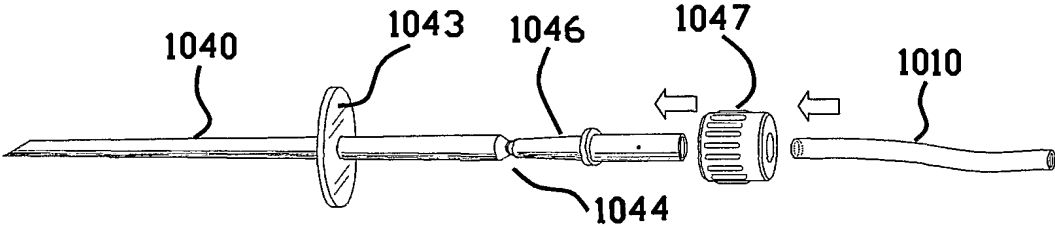


FIG. 26a

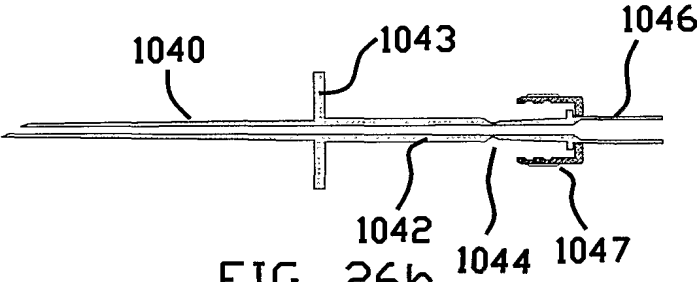


FIG. 26b

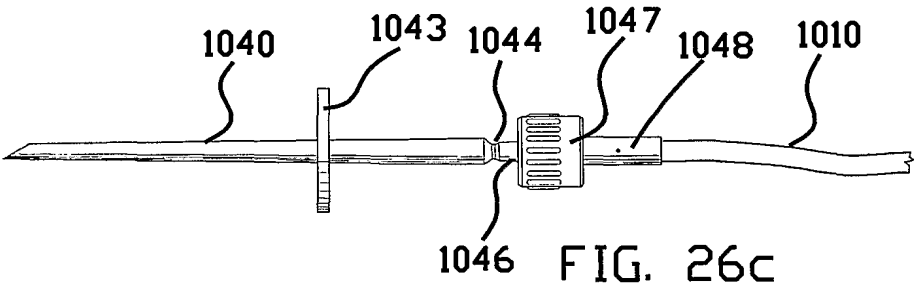


FIG. 26c

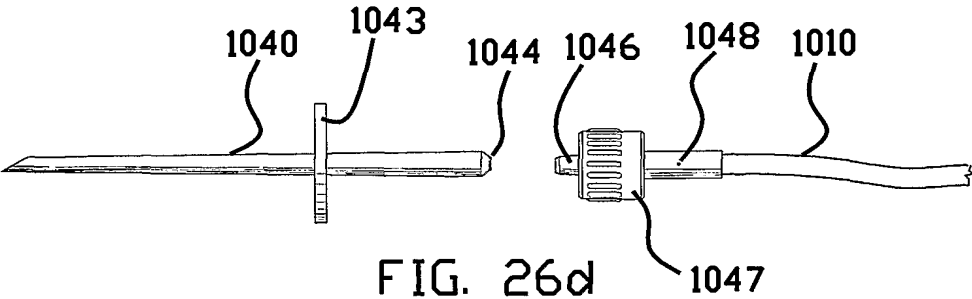
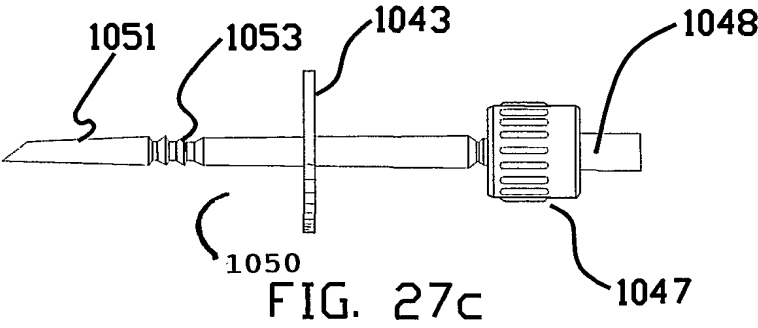
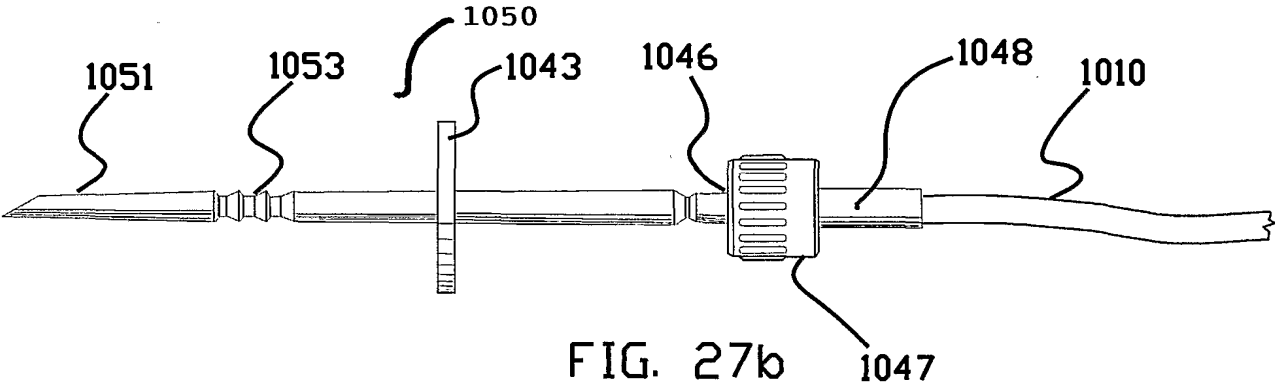
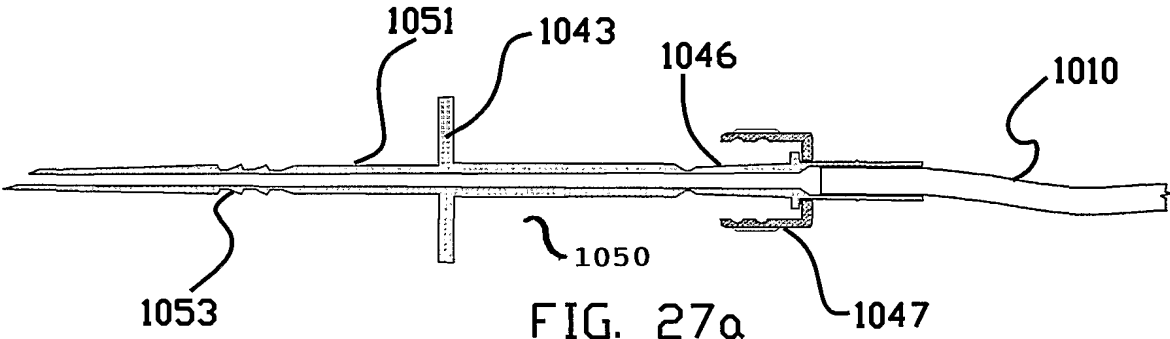
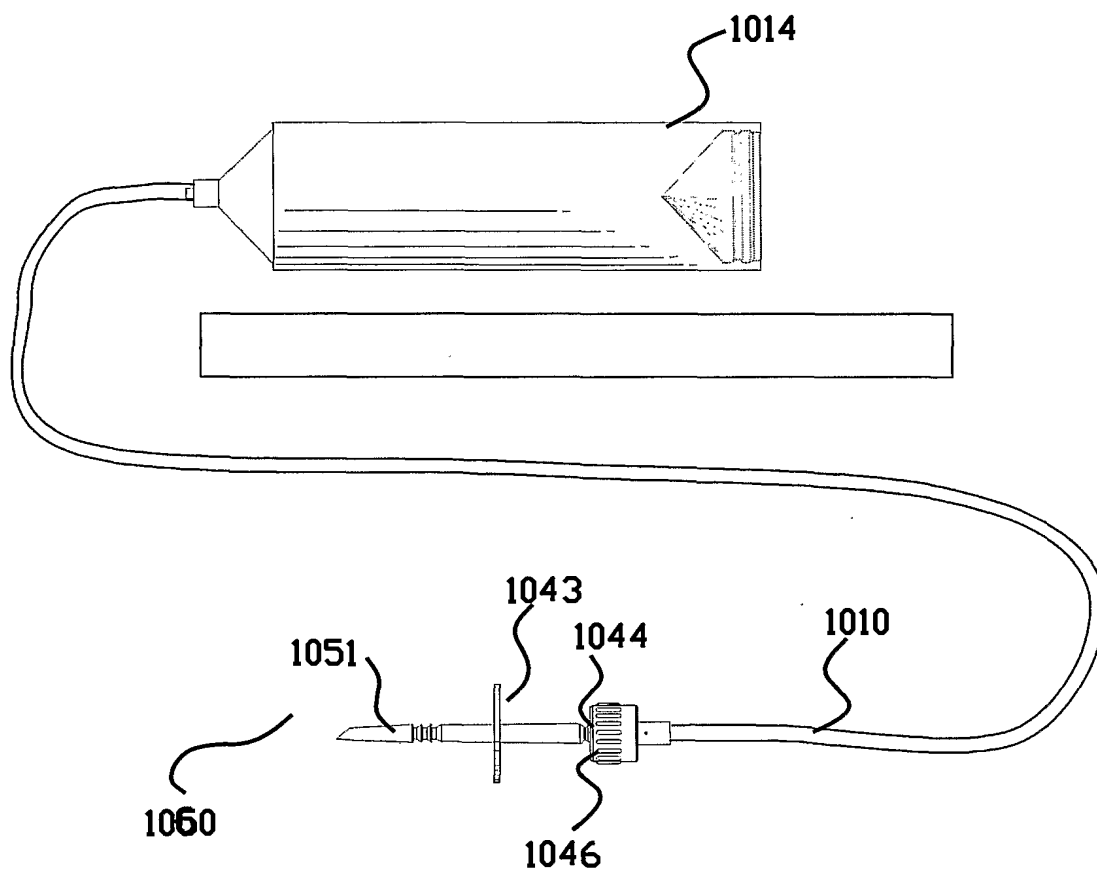
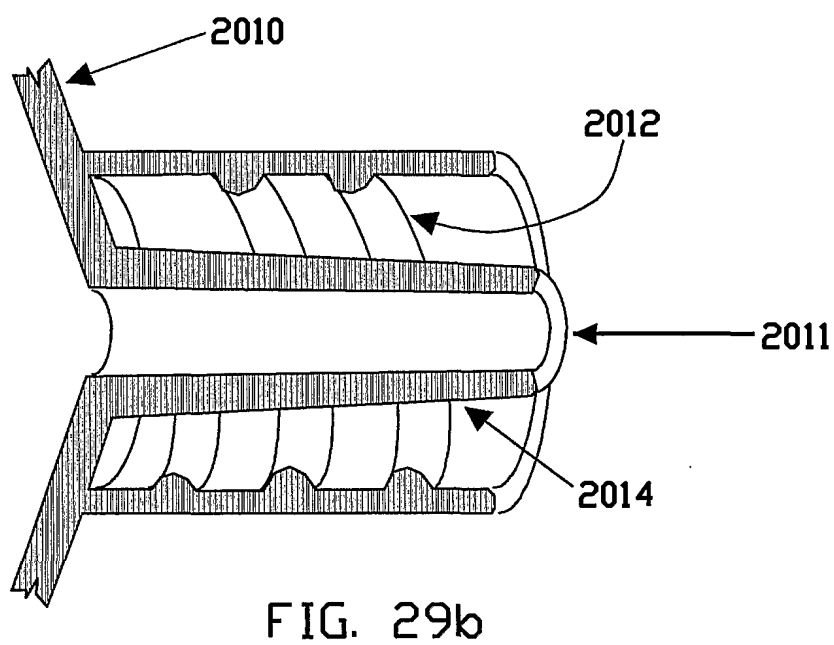
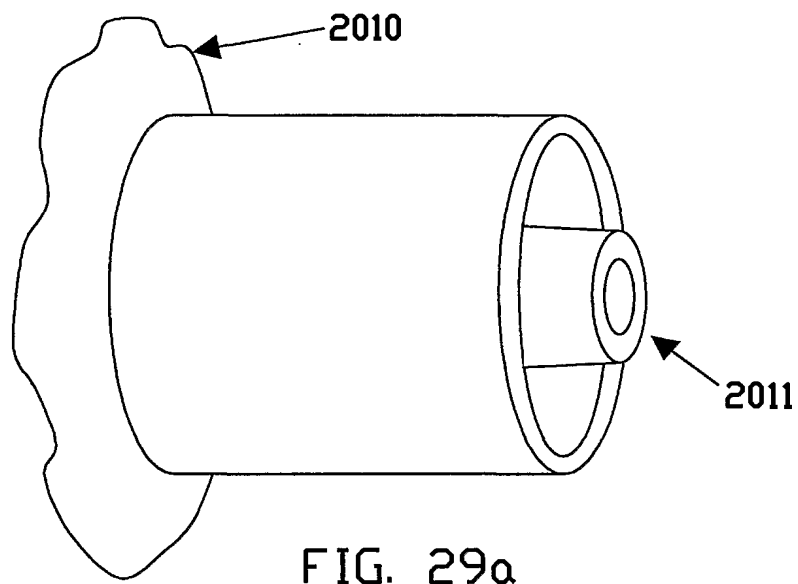


FIG. 26d







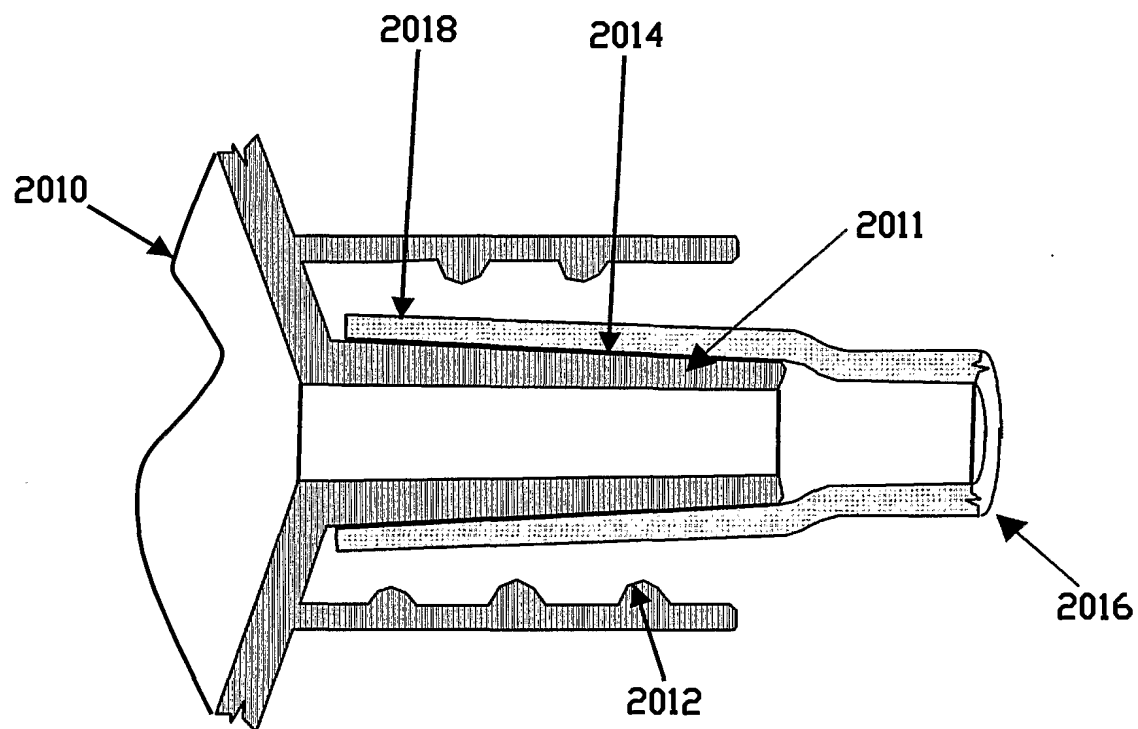
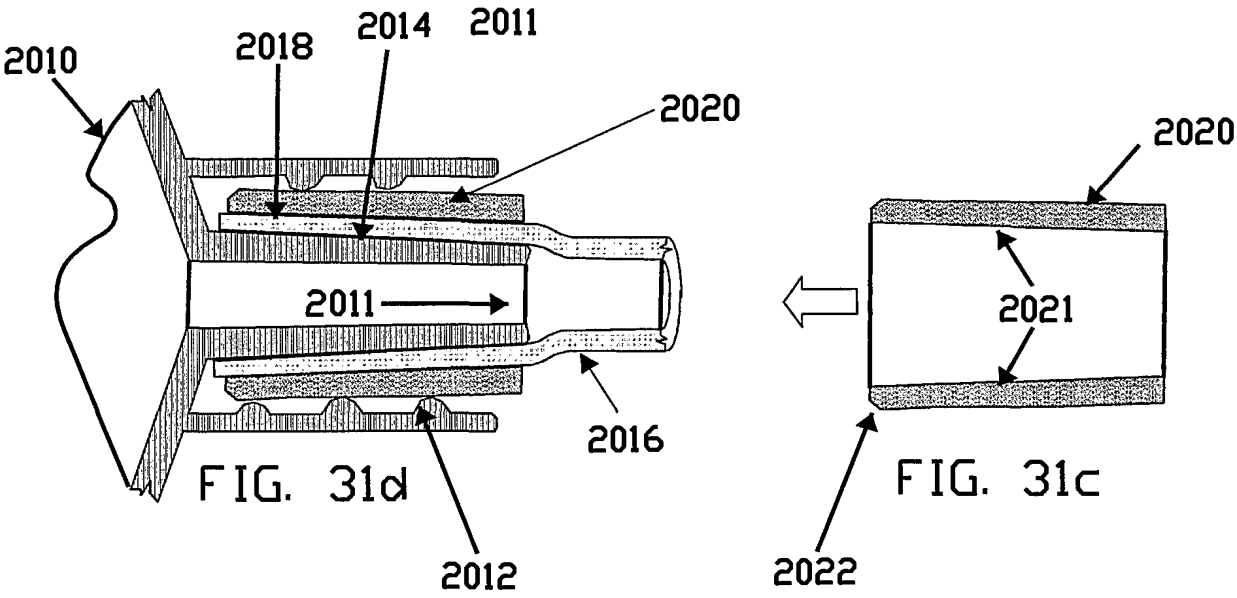
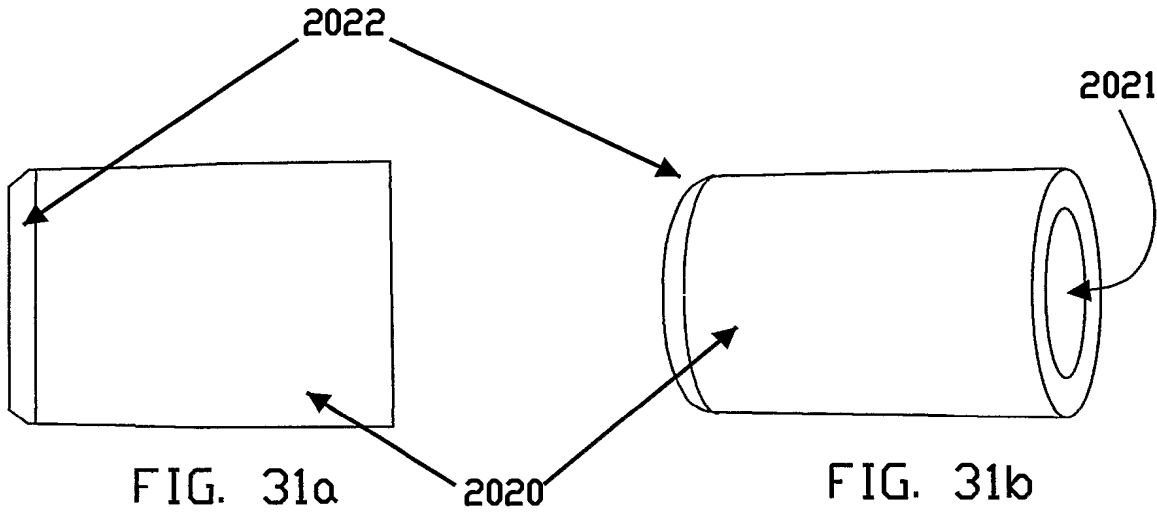


FIG. 30



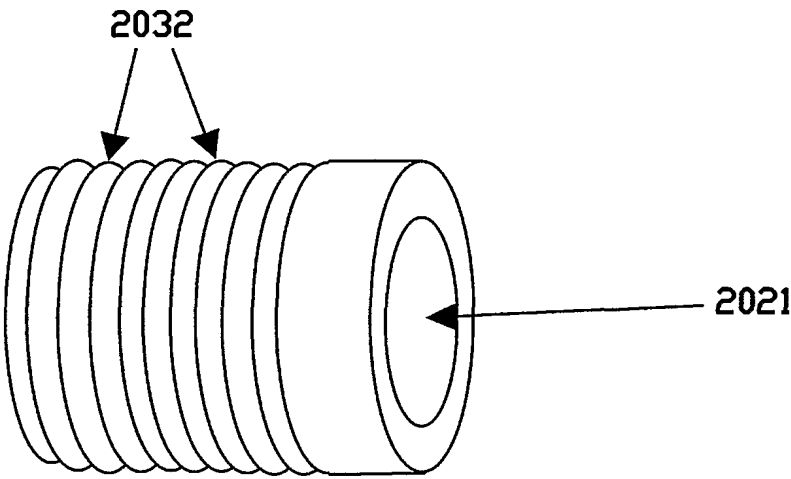


FIG. 32a

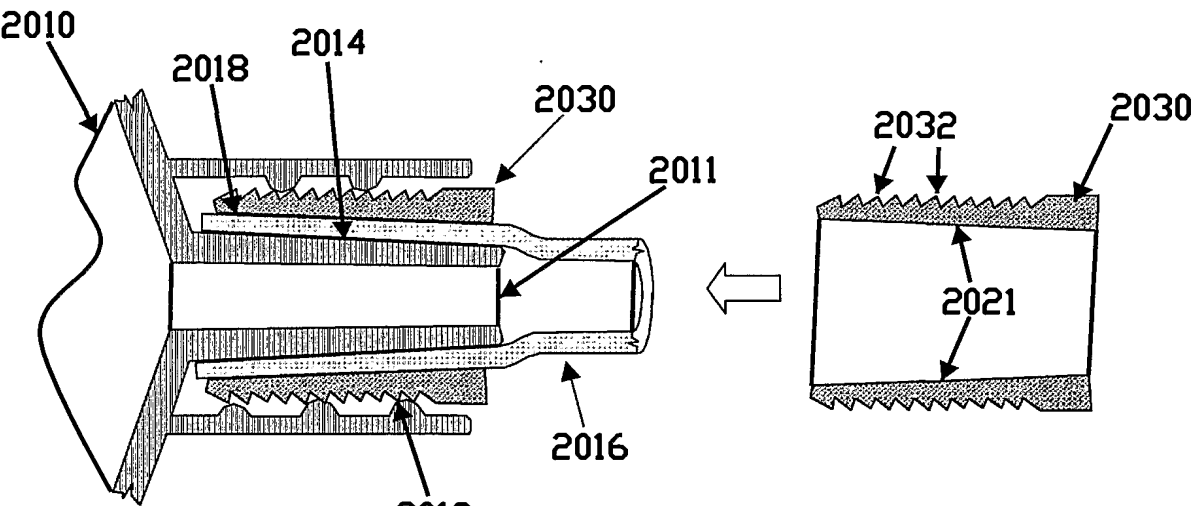
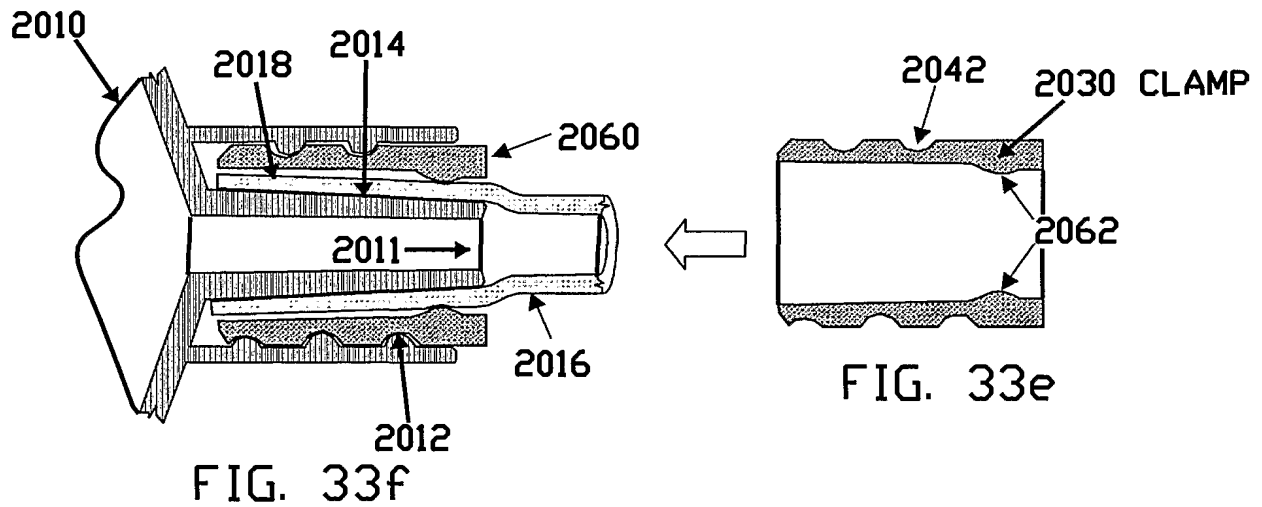
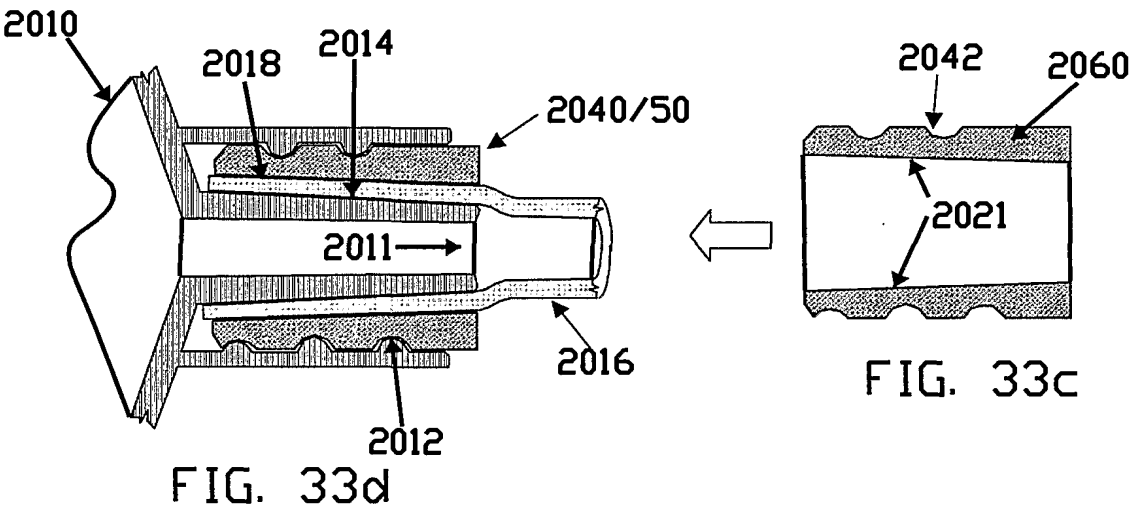
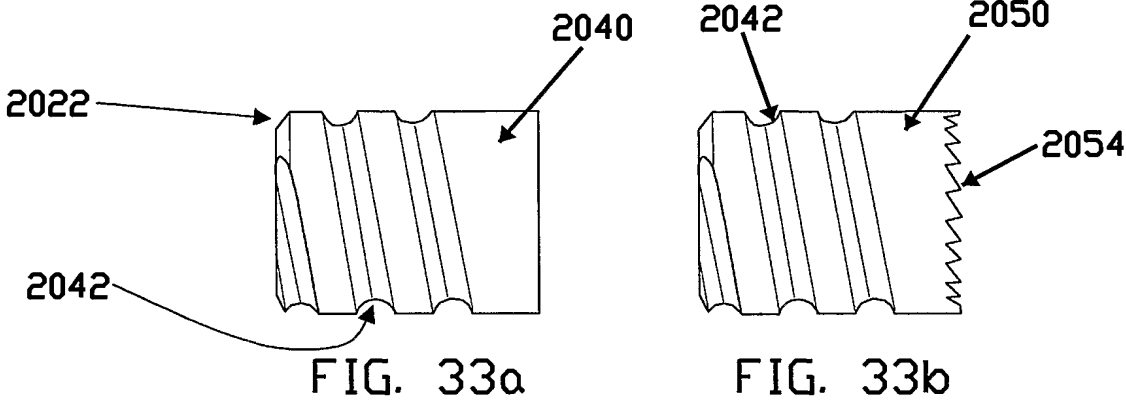
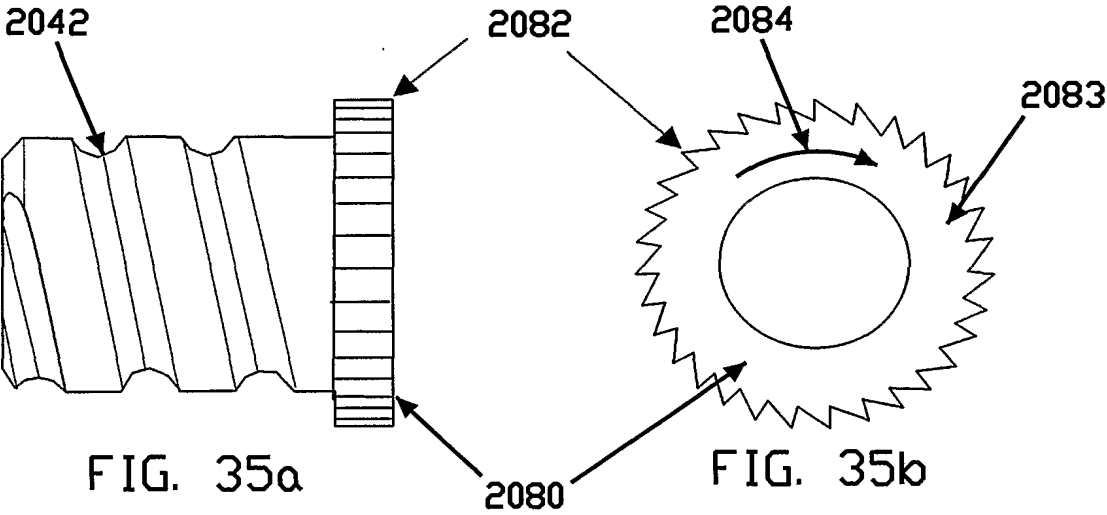
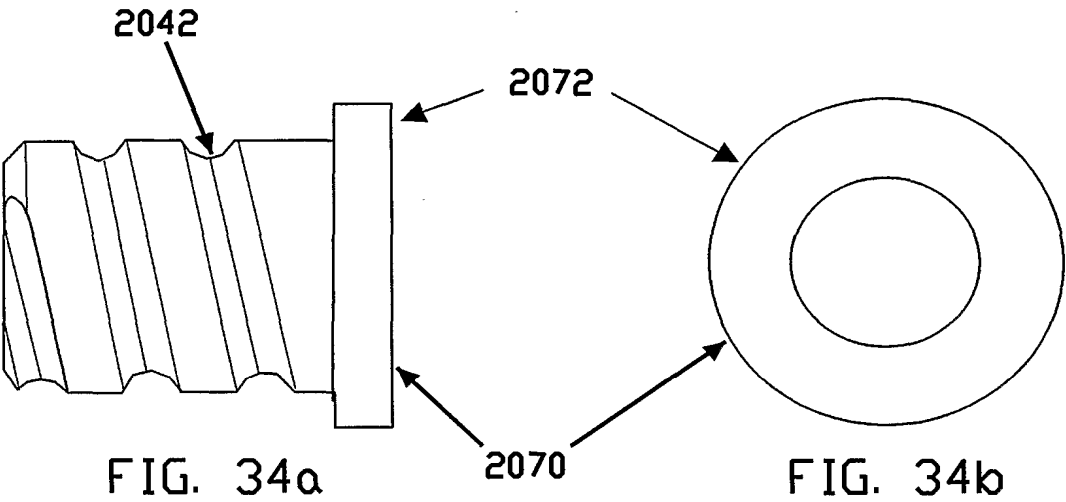


FIG. 32c

FIG. 32b





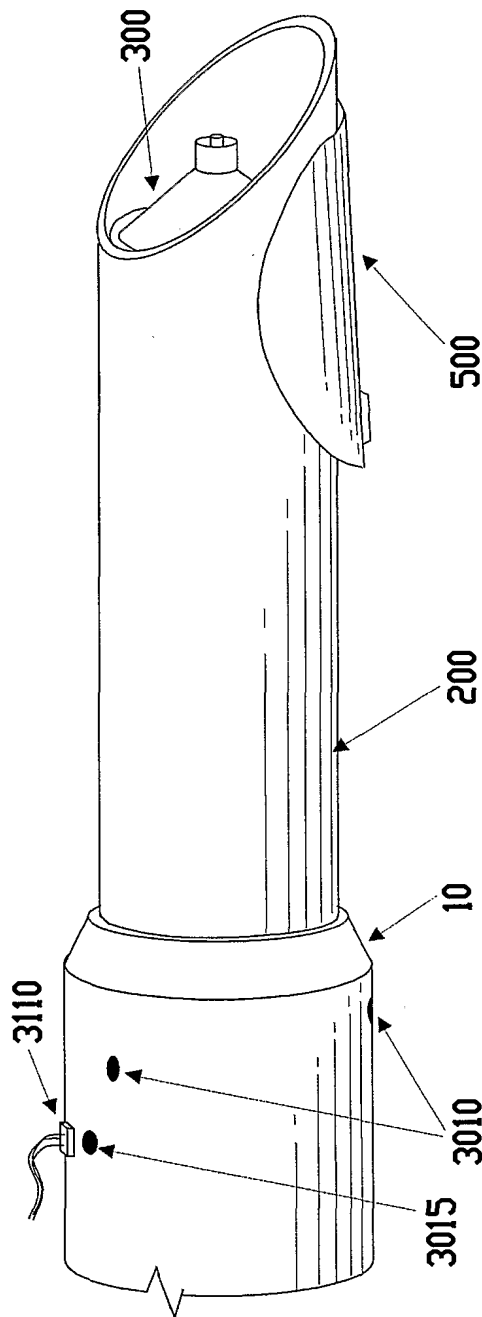
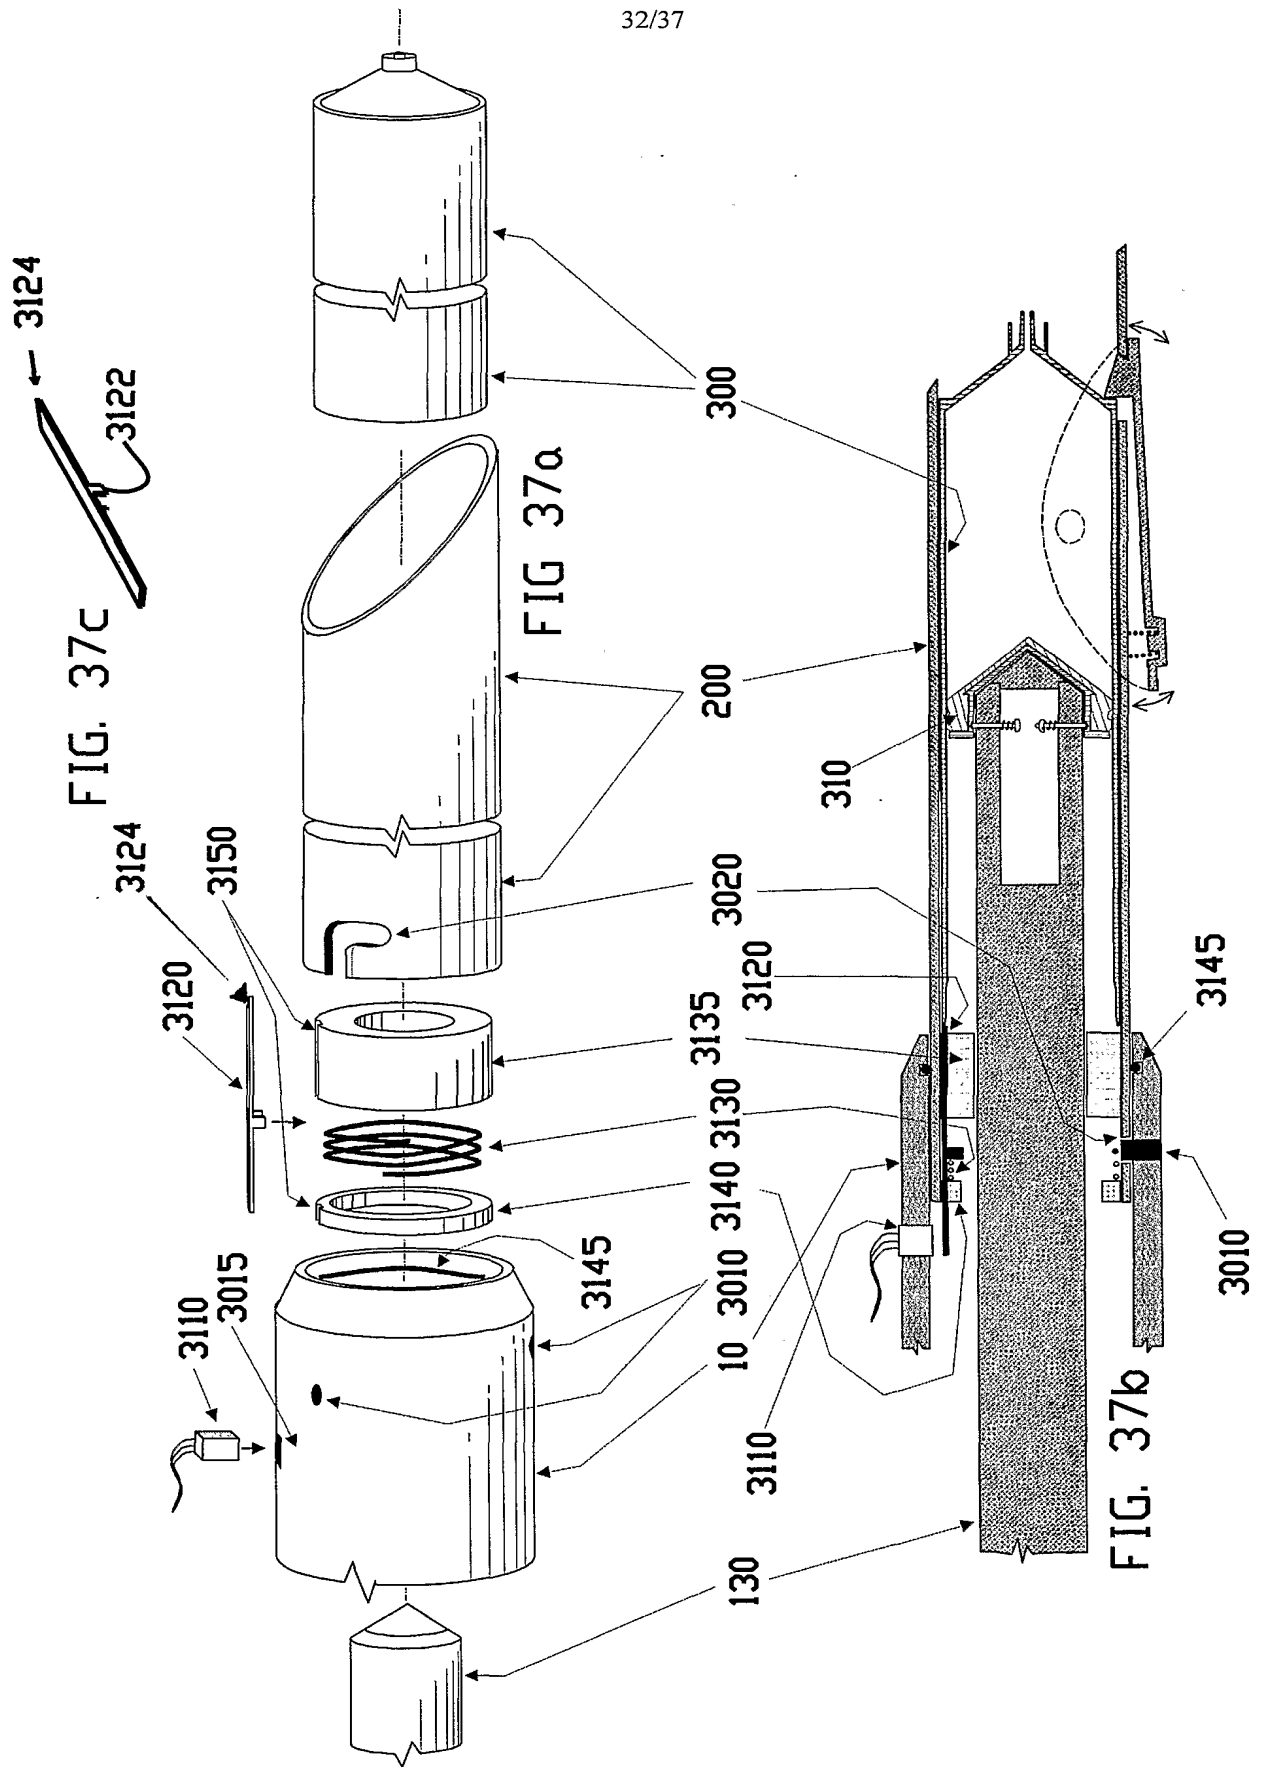


FIG. 36

32/37



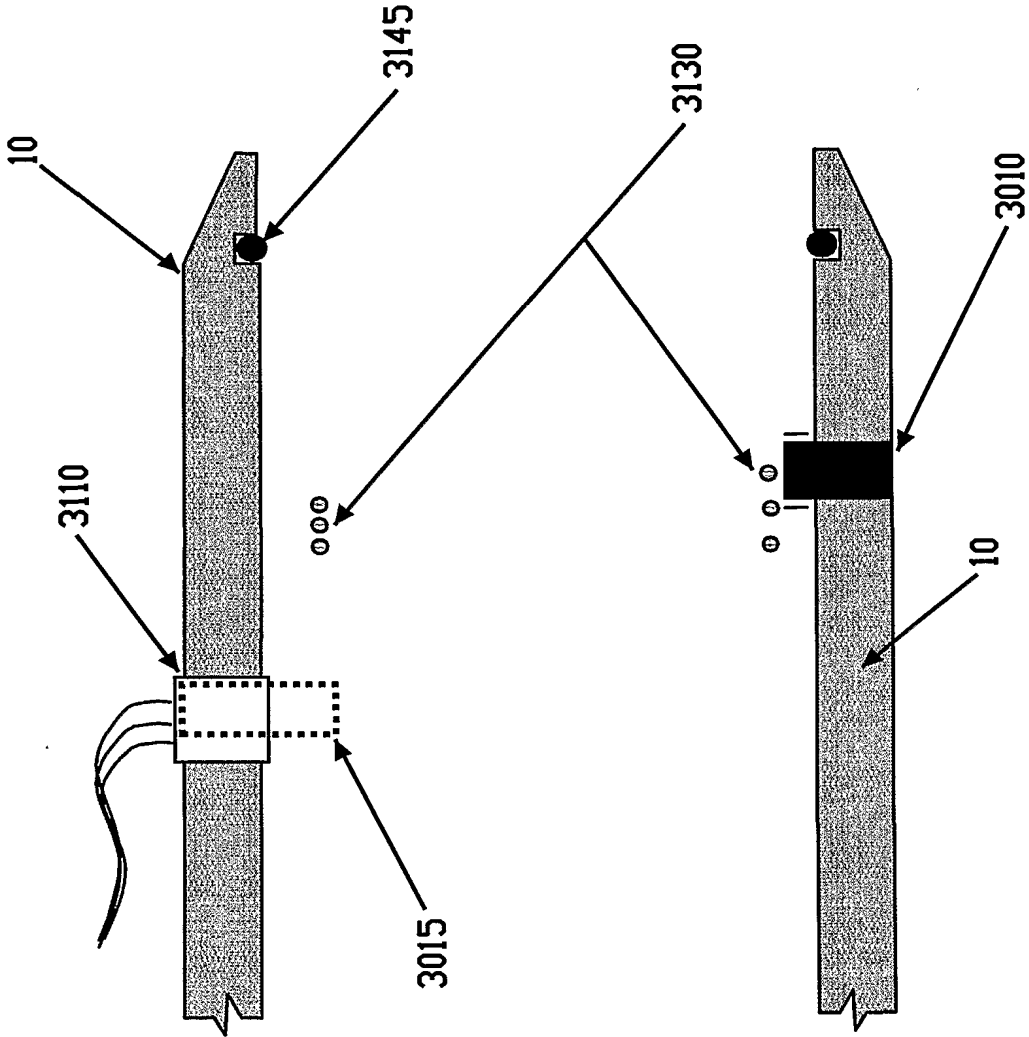


FIG. 37d

FIG. 38e



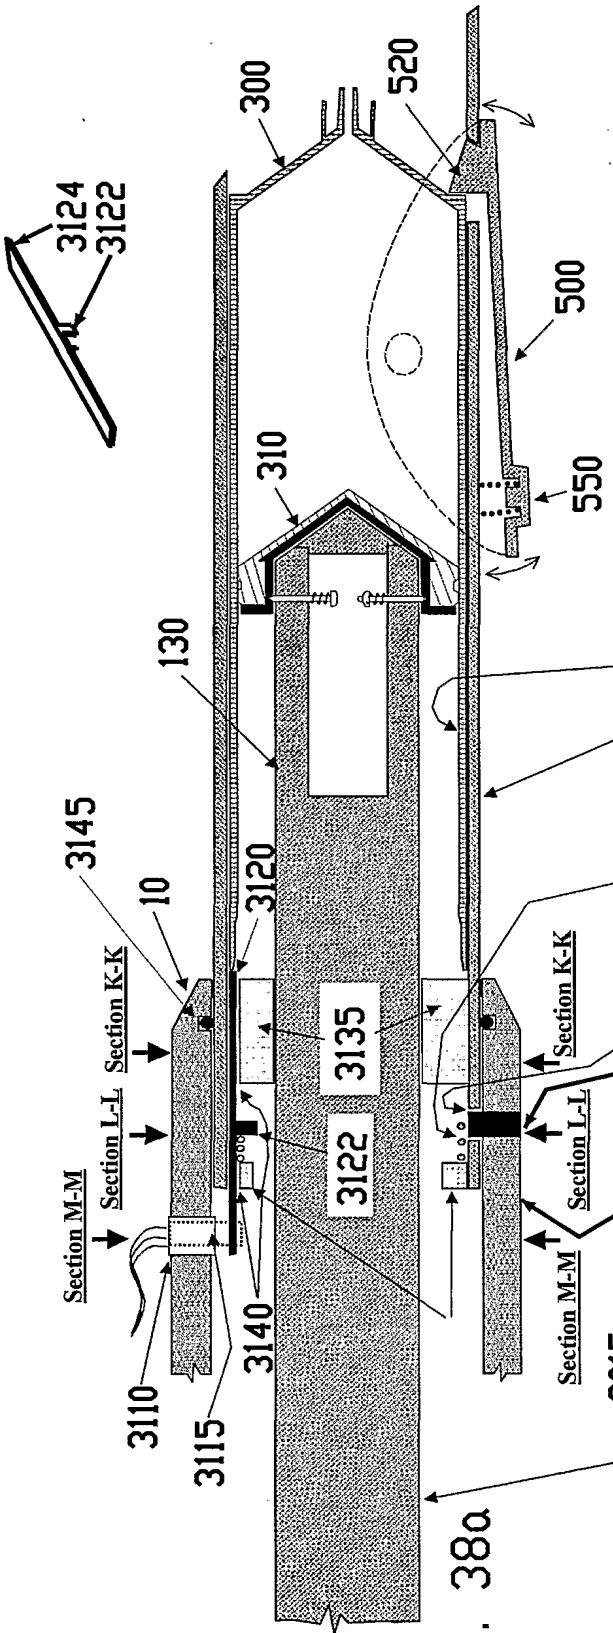


FIG. 38a

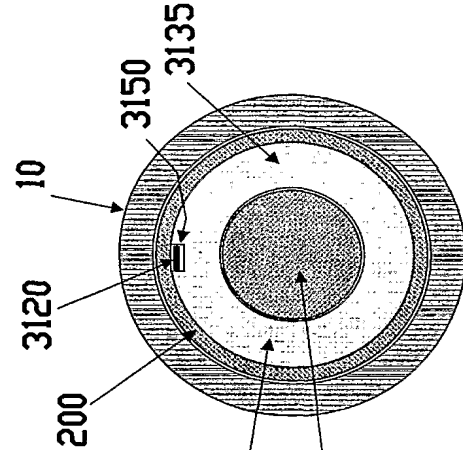


Section K-K:

FIG. 38d

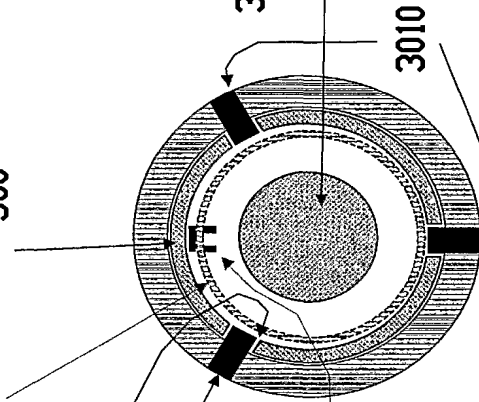



Section L-L

FIG. 38c

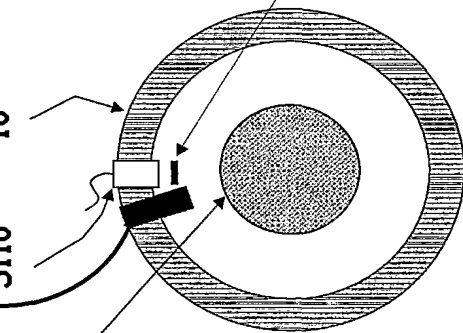

Section M-M

FIG. 38b

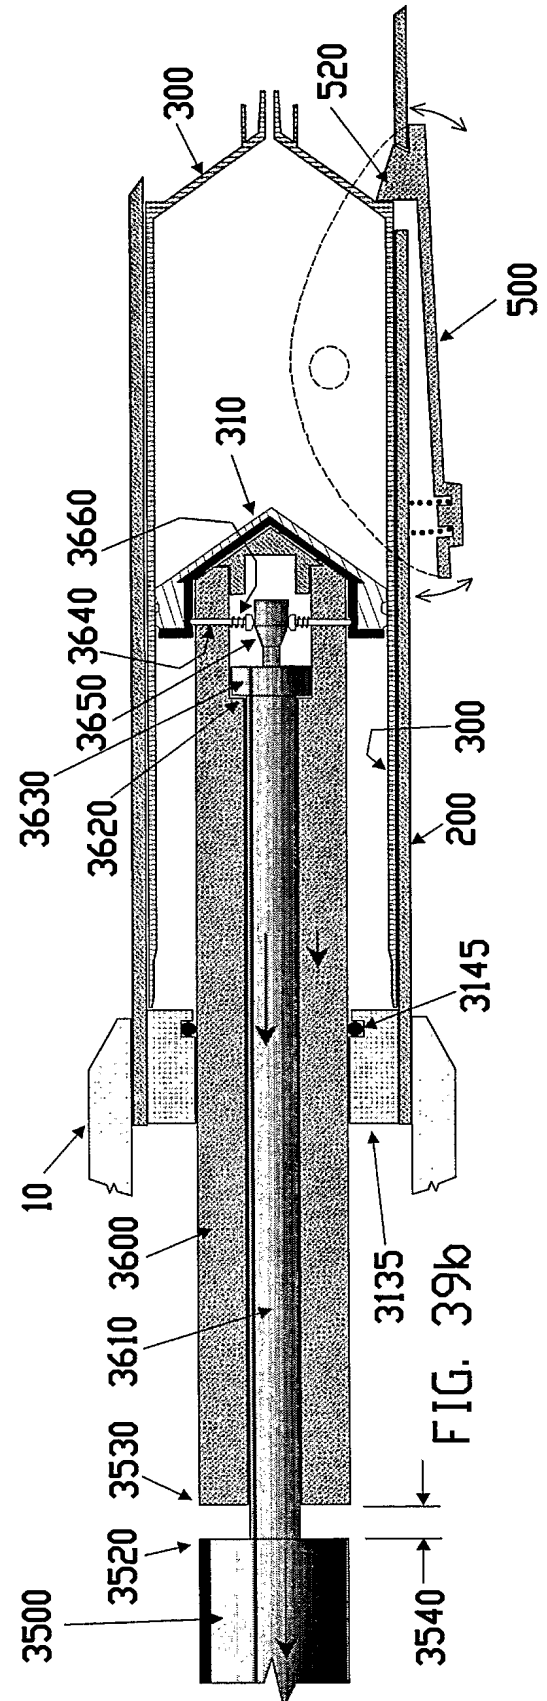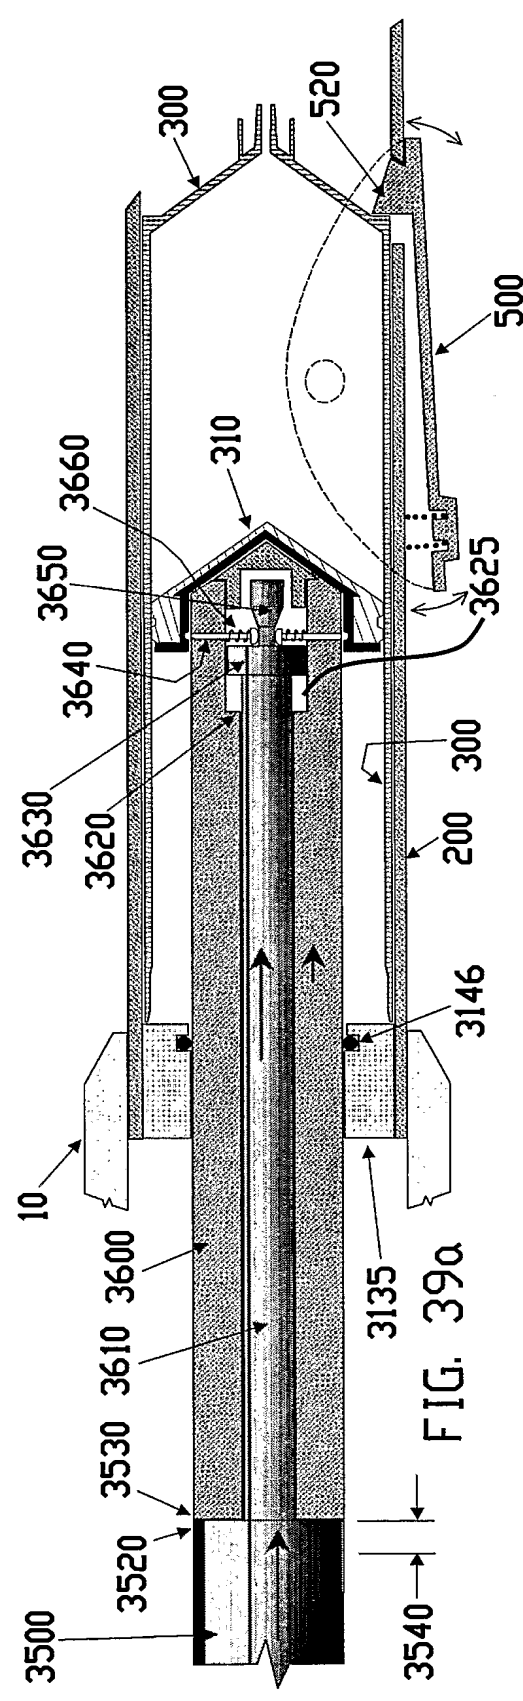



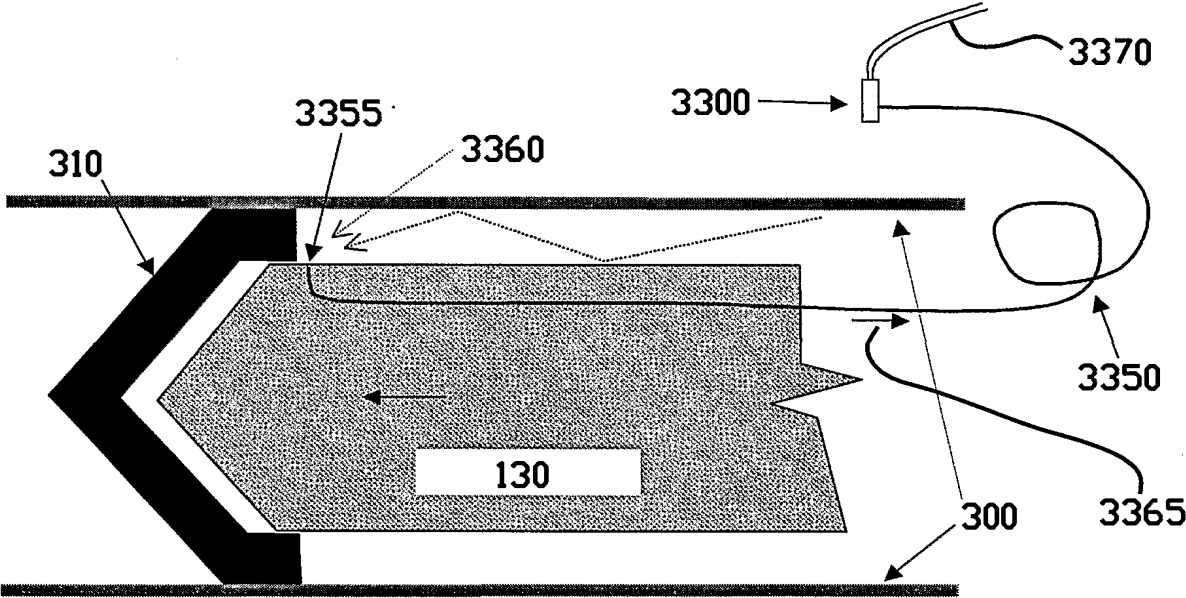


FIG. 40

37/37

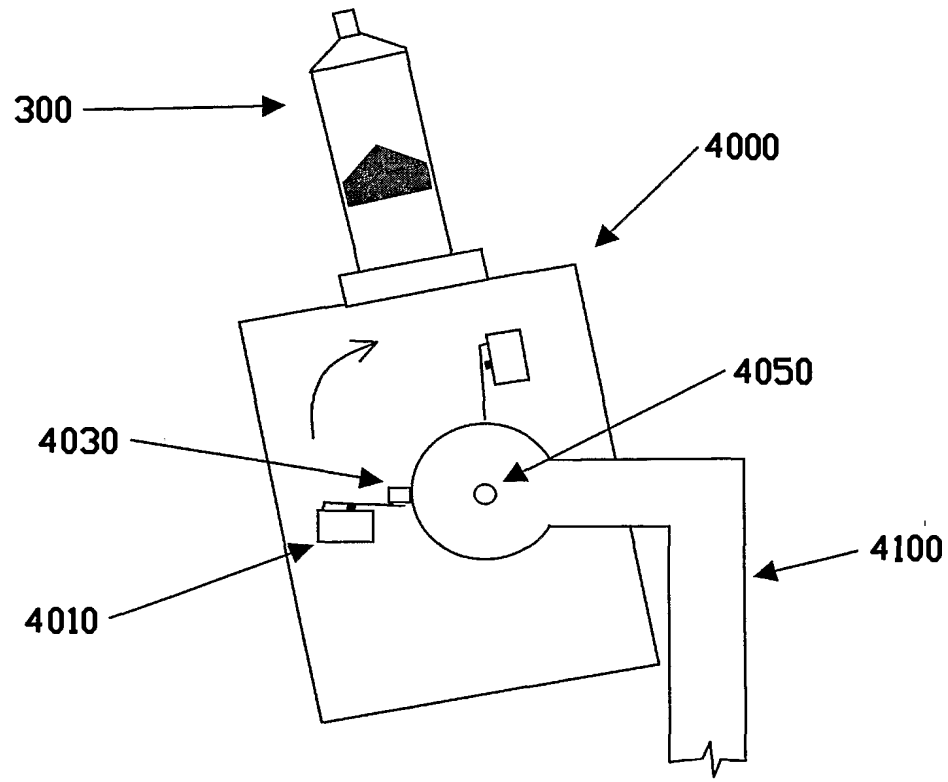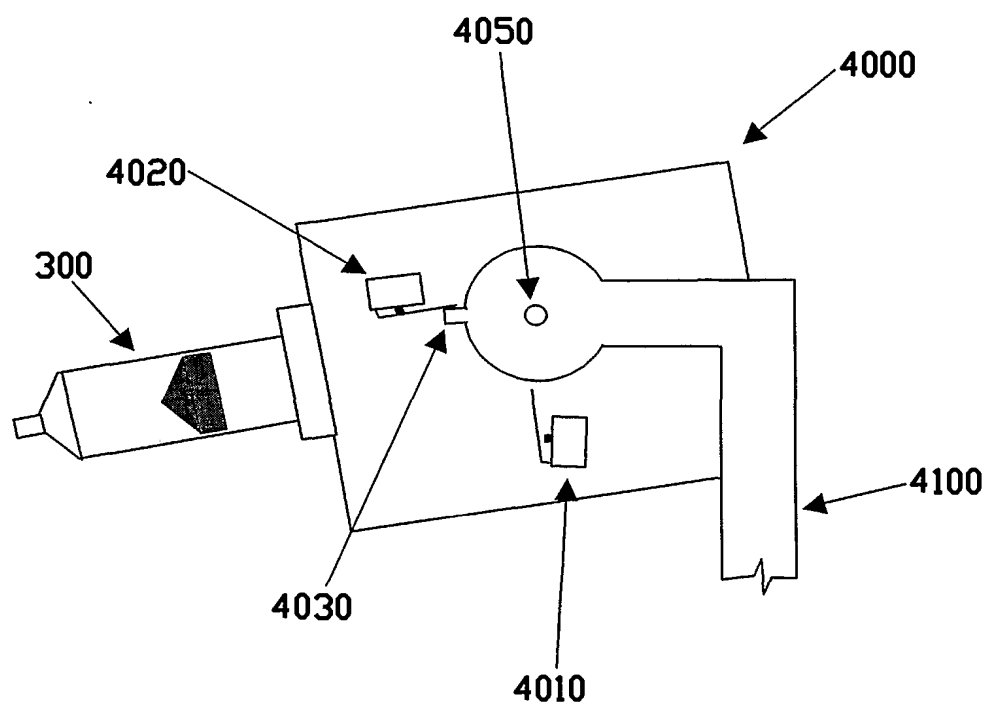

INTERNATIONAL SEARCH REPORT

International application No.

PCT/AU01/00830

A. CLASSIFICATION OF SUBJECT MATTER																						
Int. Cl. ⁷ : A61M 5/20, A61M 5/315																						
According to International Patent Classification (IPC) or to both national classification and IPC																						
B. FIELDS SEARCHED																						
Minimum documentation searched (classification system followed by classification symbols) IPC: A61M 5/20, 5/315																						
Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched AU: IPC AS ABOVE																						
Electronic data base consulted during the international search (name of data base and, where practicable, search terms used) DWPI																						
C. DOCUMENTS CONSIDERED TO BE RELEVANT																						
Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.																				
X	US 5429611A (Rait) 4 July 1995	1-4,6-9,11-18,33,34,36,183-190,251																				
X	US 5433712A (Stiles et al.) 18 July 1995	1-4,6,7																				
X	US 5106379A (Leap) 21 April 1992	1-4,7																				
<input checked="" type="checkbox"/> Further documents are listed in the continuation of Box C <input checked="" type="checkbox"/> See patent family annex																						
<p>* Special categories of cited documents:</p> <table border="0"> <tr> <td>"A"</td> <td>document defining the general state of the art which is not considered to be of particular relevance</td> <td>"T"</td> <td>later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention</td> </tr> <tr> <td>"E"</td> <td>earlier application or patent but published on or after the international filing date</td> <td>"X"</td> <td>document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone</td> </tr> <tr> <td>"L"</td> <td>document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)</td> <td>"Y"</td> <td>document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art</td> </tr> <tr> <td>"O"</td> <td>document referring to an oral disclosure, use, exhibition or other means</td> <td>"&"</td> <td>document member of the same patent family</td> </tr> <tr> <td>"P"</td> <td>document published prior to the international filing date but later than the priority date claimed</td> <td></td> <td></td> </tr> </table>			"A"	document defining the general state of the art which is not considered to be of particular relevance	"T"	later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention	"E"	earlier application or patent but published on or after the international filing date	"X"	document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone	"L"	document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)	"Y"	document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art	"O"	document referring to an oral disclosure, use, exhibition or other means	"&"	document member of the same patent family	"P"	document published prior to the international filing date but later than the priority date claimed		
"A"	document defining the general state of the art which is not considered to be of particular relevance	"T"	later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention																			
"E"	earlier application or patent but published on or after the international filing date	"X"	document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone																			
"L"	document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)	"Y"	document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art																			
"O"	document referring to an oral disclosure, use, exhibition or other means	"&"	document member of the same patent family																			
"P"	document published prior to the international filing date but later than the priority date claimed																					
Date of the actual completion of the international search 26 October 2001		Date of mailing of the international search report - 1 NOV 2001																				
Name and mailing address of the ISA/AU AUSTRALIAN PATENT OFFICE PO BOX 200, WODEN ACT 2606, AUSTRALIA E-mail address: pct@ipaustalia.gov.au Facsimile No. (02) 6285 3929		Authorized officer JON MILLS Telephone No : (02) 6283 2113																				

INTERNATIONAL SEARCH REPORT

International application No.

PCT/AU01/00830

C (Continuation). DOCUMENTS CONSIDERED TO BE RELEVANT		
Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	US 5007904A (Densmore et al.) 16 April 1991	43-51,60- 63,74- 75,77,85,96- 99,154,155
X	US 4677980A (Reilly et al.) 7 July 1987	43-51,60- 63,74- 75,77,85,96- 99,154,155
A	GB 2108852A (Greater Glasgow Health Board)	43

INTERNATIONAL SEARCH REPORT

International application No.

PCT/AU01/00830

Box I Observations where certain claims were found unsearchable (Continuation of item 2 of first sheet)

This international search report has not been established in respect of certain claims under Article 17(2)(a) for the following reasons:

1. ☐ Claims Nos :
because they relate to subject matter not required to be searched by this Authority, namely:
2. ☒ Claims Nos : 271-277
because they relate to parts of the international application that do not comply with the prescribed requirements to such an extent that no meaningful international search can be carried out, specifically:
They are not in accordance with Rule 6.2(a)
3. ☒ Claims Nos : 22-29,38-42,52-59,66-73,88-95,102-108,115-122,129-135,148-152,156,165,180,209-212,228,244,252-255 and 265-268
because they are dependent claims and are not drafted in accordance with the second and third sentences of Rule 6.4(a)

Box II Observations where unity of invention is lacking (Continuation of item 3 of first sheet)

This International Searching Authority found multiple inventions in this international application, as follows:

See extra sheet.

1. ☐ As all required additional search fees were timely paid by the applicant, this international search report covers all searchable claims
2. ☐ As all searchable claims could be searched without effort justifying an additional fee, this Authority did not invite payment of any additional fee.
3. ☒ As only some of the required additional search fees were timely paid by the applicant, this international search report covers only those claims for which fees were paid, specifically claims Nos.:
1-21,30-37,163,164,174,175,183-208,213-227,248-251 and 256-264 and
43-51,60-65,74-87,96-101,154 and 155
4. ☐ No required additional search fees were timely paid by the applicant. Consequently, this international search report is restricted to the invention first mentioned in the claims; it is covered by claims Nos.:

Remark on Protest

☐ The additional search fees were accompanied by the applicant's protest.

☒ No protest accompanied the payment of additional search fees.

Supplemental Box

(To be used when the space in any of Boxes I to VIII is not sufficient)

Continuation of Box No: II

The international application does not comply with the requirements of unity of invention because it does not relate to one invention or to a group of inventions so linked as to form a single general inventive concept. In coming to this conclusion the International Searching Authority has found that there are different inventions as follows:

1. Claims 1-21,30-37,163,164,174,175,183-208,213-227,248-251 and 256-264 are directed to an injector system with a syringe holder which releasably locks a syringe in place with a pivotable catch. It is considered that this catch comprises a first "special technical feature".
2. Claims 43-51,60-65,154,74-87,96-101 and 155 are directed to a hub and plunger for a syringe which are releasably engaged via a substantially annular engaging portion on the hub so that the hub may be withdrawn by the plunger. It is considered that this annular engaging portion comprises a second "special technical feature".
3. Claims 109-114,123-128 are directed to a syringe which has a hub and plunger which are releasably interengaged and a sensor to detect the level of engagement. It is considered that this sensor comprises a third "special technical feature".
4. Claims 136-147 are directed to a device for manually filling a syringe which has a hub and plunger which are releasably interengaged. It is considered that this filling device comprises a fourth "special technical feature".
5. Claims 157-162,182,269 are directed to a sensing system to detect the presence of a syringe holder associated with an injector system. It is considered that this sensing system comprises a fifth "special technical feature".
6. Claims 166-173,176-179,181,270 are directed to a sensing system to detect the presence of a syringe in a syringe holder. It is considered that this sensing system comprises a sixth "special technical feature".
7. Claims 245-247 are directed to a method of filling a syringe. It is considered that this method comprises a seventh "special technical feature".

Since the abovementioned groups of claims do not share any of the technical features identified, a "technical relationship" between the inventions, as defined in PCT rule 13.2 does not exist. Accordingly the international application does not relate to one invention or to a single inventive concept, a priori.

INTERNATIONAL SEARCH REPORT
Information on patent family members

International application No.
PCT/AU01/00830

This Annex lists the known "A" publication level patent family members relating to the patent documents cited in the above-mentioned international search report. The Australian Patent Office is in no way liable for these particulars which are merely given for the purpose of information.

Patent Document Cited in Search Report		Patent Family Member
US	5429611	NO FAMILY
US	5433712	NO FAMILY
US	5106379	NO FAMILY
US	5007904	NO FAMILY
US	4677980	NO FAMILY

END OF ANNEX